

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018727.D
 Acq On : 07 Oct 2020 14:01
 Operator : SY/MD
 Sample : L4287-05DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	135153	135498	12.72%	1.466%
2	1.579	145	152	167	rVB	126841	142570	13.39%	1.543%
3	2.122	312	321	349	rVB	244996	381522	35.83%	4.128%
4	2.781	518	526	537	rVB9	4330	7244	0.68%	0.078%
5	2.839	541	544	547	rBV2	744	485	0.05%	0.005%
6	2.862	548	551	555	rVB2	431	300	0.03%	0.003%
7	2.894	557	561	563	rBV2	531	369	0.03%	0.004%
8	3.061	609	613	618	rVB5	679	726	0.07%	0.008%
9	3.116	624	630	632	rBV3	780	710	0.07%	0.008%
10	3.273	676	679	683	rBV2	402	334	0.03%	0.004%
11	3.576	767	773	776	rBV3	467	373	0.04%	0.004%
12	3.598	776	780	784	rVB3	531	380	0.04%	0.004%
13	3.621	784	787	791	rBV2	472	462	0.04%	0.005%
14	3.708	812	814	820	rVB3	499	440	0.04%	0.005%
15	3.843	854	856	859	rBV2	454	295	0.03%	0.003%
16	3.936	869	885	920	rBV3	120949	389482	36.58%	4.215%
17	4.254	982	984	988	rBV2	620	301	0.03%	0.003%
18	4.376	1003	1022	1047	rBV	157474	397372	37.32%	4.300%
19	4.595	1086	1090	1094	rVB4	828	720	0.07%	0.008%
20	4.617	1094	1097	1099	rBV2	557	426	0.04%	0.005%
21	4.720	1125	1129	1130	rBV2	602	397	0.04%	0.004%
22	4.843	1164	1167	1172	rVB2	441	427	0.04%	0.005%
23	4.913	1187	1189	1193	rBV4	595	448	0.04%	0.005%
24	5.071	1222	1238	1261	rBV2	381636	986425	92.63%	10.674%
25	5.489	1365	1368	1377	rVB6	787	1113	0.10%	0.012%
26	5.531	1377	1381	1382	rBV2	660	345	0.03%	0.004%
27	5.640	1403	1415	1439	rBV	340212	682872	64.13%	7.389%
28	5.936	1489	1507	1530	rBV5	125251	290056	27.24%	3.139%
29	6.093	1544	1556	1585	rVB	223003	449353	42.20%	4.862%
30	6.277	1609	1613	1616	rBV4	666	627	0.06%	0.007%
31	6.318	1624	1626	1632	rVB5	875	606	0.06%	0.007%
32	6.431	1658	1661	1663	rVB2	647	363	0.03%	0.004%
33	6.604	1711	1715	1717	rBV2	471	407	0.04%	0.004%
34	6.627	1720	1722	1725	rBV4	401	313	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018727.D
 Acq On : 07 Oct 2020 14:01
 Operator : SY/MD
 Sample : L4287-05DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

35	6.659	1730	1732	1735	rBV	812	676	0.06%	0.007%
36	6.900	1804	1807	1811	rVB2	549	447	0.04%	0.005%
37	6.932	1814	1817	1818	rBV2	591	311	0.03%	0.003%
38	6.965	1823	1827	1830	rBV2	804	492	0.05%	0.005%
39	7.006	1830	1840	1860	rBV	117787	216772	20.36%	2.346%
40	7.338	1930	1943	1961	rBV	440688	755722	70.97%	8.178%
41	7.643	2028	2038	2064	rBV	85554	153943	14.46%	1.666%
42	7.997	2134	2148	2167	rBV	634345	1064881	100.00%	11.523%
43	8.109	2174	2183	2221	rBV2	178129	380514	35.73%	4.118%
44	8.424	2278	2281	2284	rBV2	1115	740	0.07%	0.008%
45	8.473	2294	2296	2299	rBV2	492	407	0.04%	0.004%
46	8.543	2316	2318	2323	rVB3	605	381	0.04%	0.004%
47	8.669	2355	2357	2361	rVB3	1283	770	0.07%	0.008%
48	8.691	2361	2364	2367	rBV2	808	543	0.05%	0.006%
49	8.871	2409	2420	2446	rBV	531682	866503	81.37%	9.376%
50	9.103	2485	2492	2500	rVB7	969	1510	0.14%	0.016%
51	9.164	2507	2511	2512	rBV2	833	454	0.04%	0.005%
52	9.331	2558	2563	2566	rBV5	665	838	0.08%	0.009%
53	9.399	2582	2584	2587	rVB3	839	355	0.03%	0.004%
54	9.479	2606	2609	2611	rVB2	512	286	0.03%	0.003%
55	9.746	2690	2692	2694	rBV2	629	301	0.03%	0.003%
56	10.003	2770	2772	2775	rVB2	719	403	0.04%	0.004%
57	10.022	2775	2778	2784	rVB3	607	571	0.05%	0.006%
58	10.055	2784	2788	2791	rBV3	635	537	0.05%	0.006%
59	10.119	2803	2808	2809	rBV2	462	343	0.03%	0.004%
60	10.183	2826	2828	2831	rVV2	994	410	0.04%	0.004%
61	10.238	2834	2845	2866	rVV	232414	366536	34.42%	3.966%
62	10.421	2899	2902	2905	rVV4	557	366	0.03%	0.004%
63	10.514	2927	2931	2933	rBV2	614	458	0.04%	0.005%
64	10.556	2939	2944	2948	rBV2	429	441	0.04%	0.005%
65	10.579	2948	2951	2954	rBV2	635	510	0.05%	0.006%
66	10.598	2954	2957	2962	rVV3	633	465	0.04%	0.005%
67	10.662	2972	2977	2978	rBV	397	318	0.03%	0.003%
68	11.003	3080	3083	3085	rBV2	478	296	0.03%	0.003%
69	11.080	3103	3107	3110	rVB3	771	466	0.04%	0.005%
70	11.132	3118	3123	3125	rBV2	592	515	0.05%	0.006%
71	11.196	3142	3143	3148	rVB2	515	302	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100720\
 Data File : VV018727.D
 Acq On : 07 Oct 2020 14:01
 Operator : SY/MD
 Sample : L4287-05DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3186	rBV	519172	798847	75.02%	8.644%
73	11.646	3271	3283	3304	rBV	474258	736168	69.13%	7.966%
74	11.759	3316	3318	3320	rBV3	839	393	0.04%	0.004%
75	11.868	3350	3352	3354	rBV	565	387	0.04%	0.004%
76	11.964	3379	3382	3385	rBV2	531	338	0.03%	0.004%
77	11.993	3387	3391	3399	rVB2	378	540	0.05%	0.006%
78	12.032	3399	3403	3405	rBV3	455	336	0.03%	0.004%
79	12.196	3450	3454	3457	rBV2	669	655	0.06%	0.007%
80	12.212	3457	3459	3462	rVV	660	394	0.04%	0.004%
81	12.328	3493	3495	3499	rBV4	462	348	0.03%	0.004%
82	12.559	3561	3567	3572	rVV4	909	809	0.08%	0.009%
83	12.633	3588	3590	3592	rBV2	763	296	0.03%	0.003%
84	12.681	3602	3605	3608	rBV2	827	587	0.06%	0.006%
85	12.701	3608	3611	3615	rBV2	608	456	0.04%	0.005%
86	12.759	3627	3629	3632	rVB2	718	309	0.03%	0.003%
87	12.807	3641	3644	3647	rVB2	730	424	0.04%	0.005%
88	12.849	3653	3657	3658	rBV2	489	331	0.03%	0.004%
89	12.939	3683	3685	3689	rVB2	796	500	0.05%	0.005%
90	12.961	3689	3692	3698	rVB4	632	670	0.06%	0.007%
91	12.990	3698	3701	3703	rBV2	700	348	0.03%	0.004%
92	13.064	3718	3724	3728	rBV3	752	861	0.08%	0.009%
93	13.087	3728	3731	3734	rVV2	688	534	0.05%	0.006%
94	13.109	3736	3738	3745	rVB4	759	546	0.05%	0.006%
95	13.482	3850	3854	3855	rBV2	370	301	0.03%	0.003%
96	13.662	3907	3910	3914	rBV	536	369	0.03%	0.004%
97	14.064	4033	4035	4041	rVB2	786	475	0.04%	0.005%
98	14.119	4050	4052	4055	rVB2	850	377	0.04%	0.004%
99	14.688	4226	4229	4232	rBV3	720	609	0.06%	0.007%
100	15.431	4457	4460	4462	rBV2	961	619	0.06%	0.007%


Sum of corrected areas: 9241371

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100720\
Data File : VV018727.D
Acq On : 07 Oct 2020 14:01
Operator : SY/MD
Sample : L4287-05DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

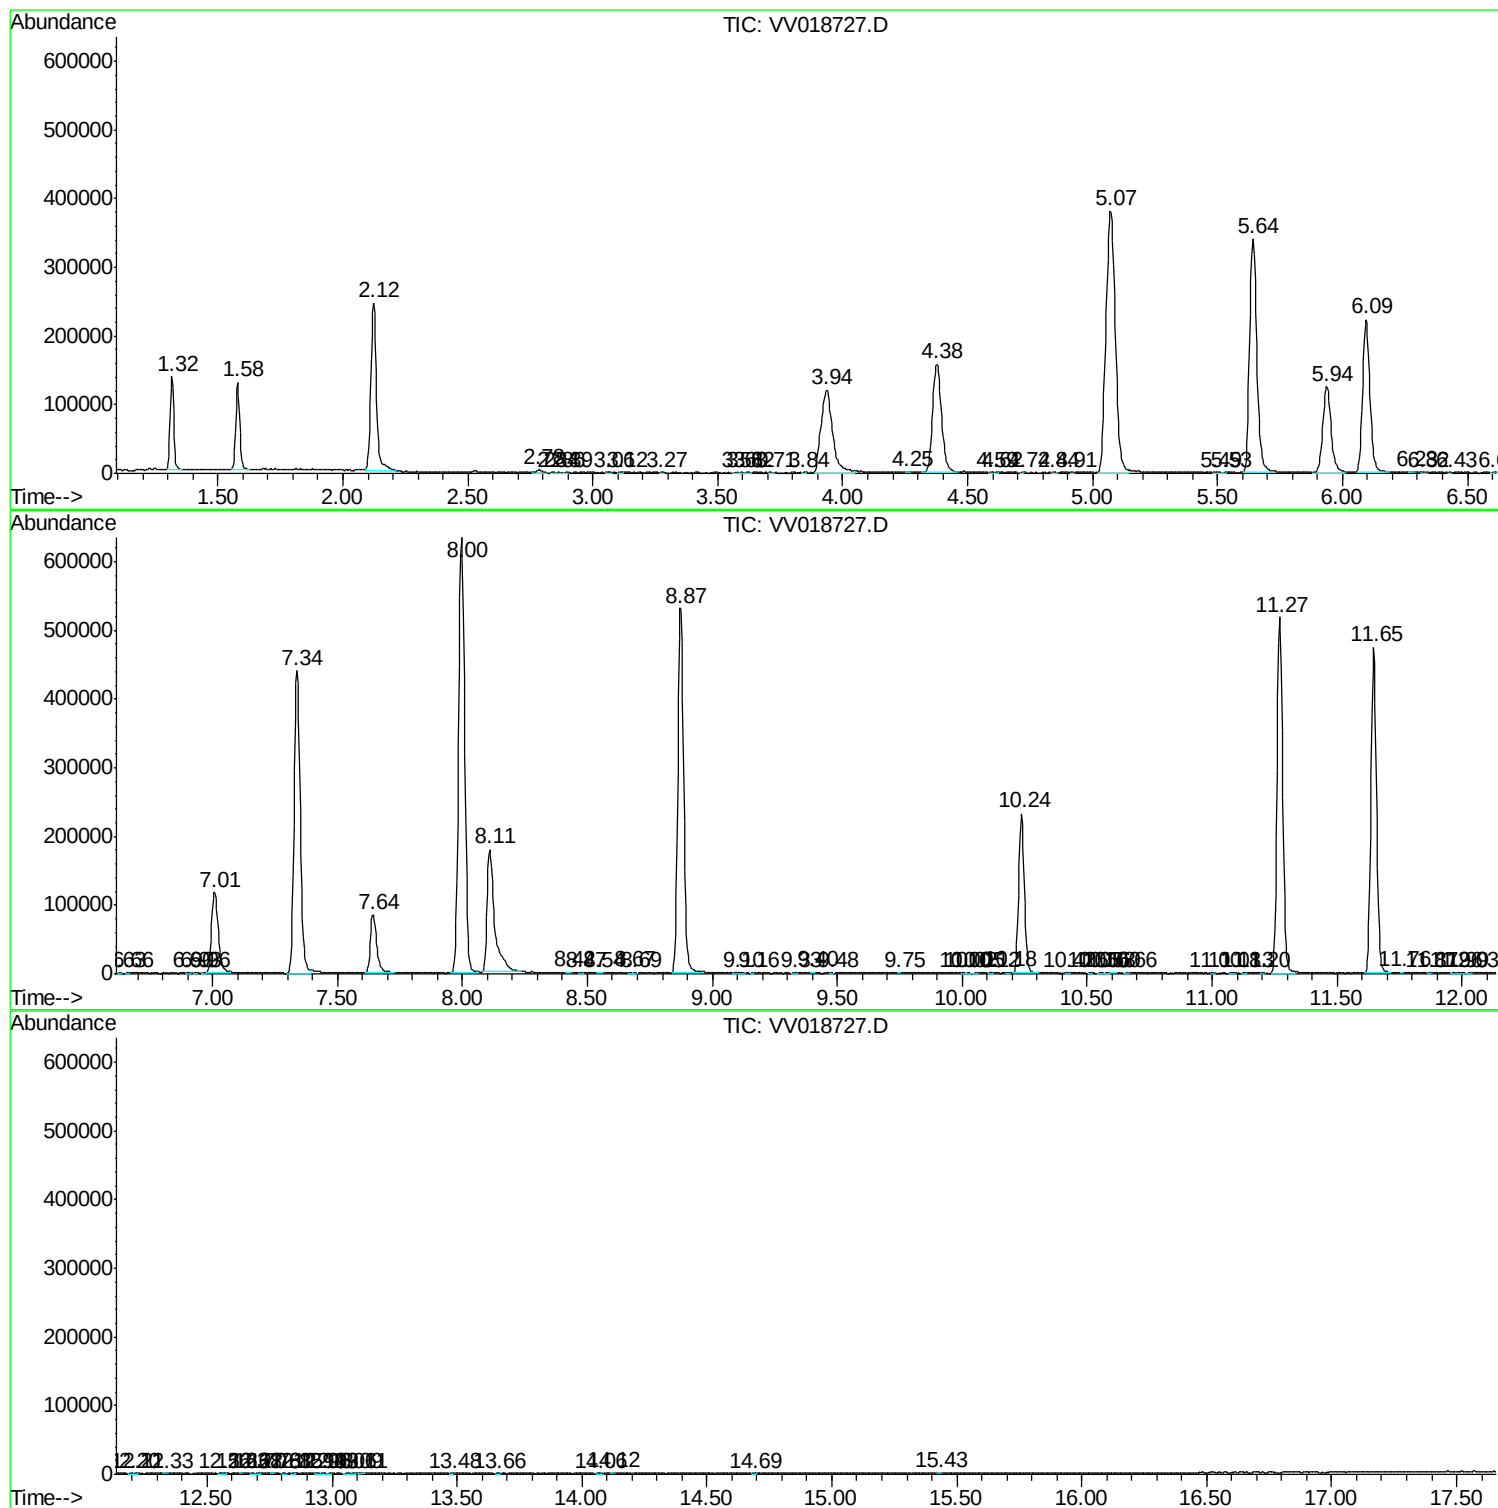

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100720\
Data File : VV018727.D
Acq On : 07 Oct 2020 14:01
Operator : SY/MD
Sample : L4287-05DL 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AK5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV100720\
Data File : VV018727.D
Acq On : 07 Oct 2020 14:01
Operator : SY/MD
Sample : L4287-05DL 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AK5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc