


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100720\
 Data File : VV018719.D
 Acq On : 07 Oct 2020 10:06
 Operator : SY/MD
 Sample : BFB69
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB69

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 07 07:22:30 2020

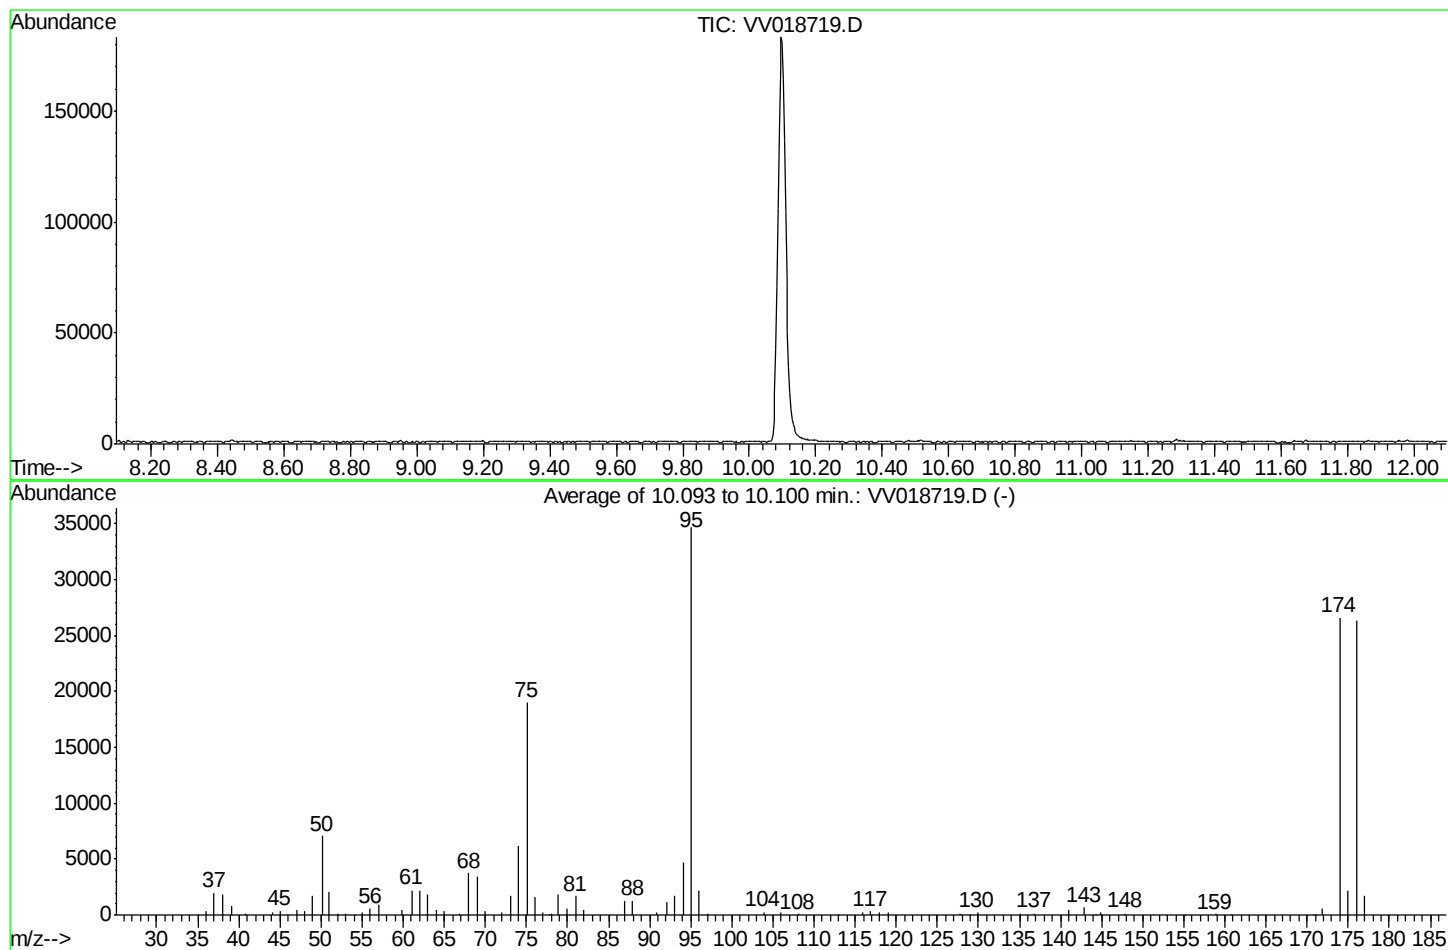

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	7068	PASS
75	95	30	80	54.7	18965	PASS
95	95	100	100	100.0	34690	PASS
96	95	5	9	6.3	2197	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.6	26578	PASS
175	174	5	9	8.4	2233	PASS
176	174	95	101	99.3	26389	PASS
177	176	5	9	6.6	1739	PASS

m/z	Abundance
36.10	350.0
37.00	1896.0
38.00	1888.0
39.00	795.0
40.00	205.0
40.90	124.0
44.00	782.0
45.00	387.0
47.00	439.0
48.00	308.0
49.00	1554.0
50.10	6917.0
51.00	2061.0
52.10	129.0
53.00	147.0
55.10	196.0
56.00	611.0
57.00	965.0
59.90	470.0
61.10	2147.0
62.00	1994.0
63.00	1910.0
64.00	410.0
65.00	341.0
66.90	182.0
68.00	3718.0
69.00	3236.0
70.00	354.0
72.00	230.0
73.10	1883.0
74.00	5915.0
75.10	18264.0
76.00	1570.0
76.90	220.0
78.00	135.0
78.90	1732.0
80.00	523.0
80.90	1638.0
81.90	411.0
87.00	1343.0
87.90	1283.0
90.90	185.0
92.10	1136.0
93.00	1749.0
94.10	4448.0
95.10	32416.0
96.00	2207.0
97.00	144.0
103.90	255.0
105.90	264.0
116.00	180.0
116.90	282.0
118.00	200.0
119.10	223.0
127.70	122.0
129.00	117.0
129.90	209.0
135.00	130.0
136.90	139.0
141.00	466.0
142.90	712.0
144.20	110.0
144.80	245.0
147.90	128.0
155.10	126.0
158.90	106.0
171.90	503.0
174.00	24960.0
175.00	2188.0
176.00	24552.0
176.90	1509.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	380.0
37.00	2064.0
38.10	1906.0
39.10	793.0
40.00	193.0
40.80	122.0
44.00	760.0
45.00	386.0
47.00	522.0
48.10	349.0
49.00	1782.0
50.10	7306.0
51.00	2130.0
52.10	181.0
53.00	187.0
55.10	228.0
56.00	533.0
57.00	981.0
59.90	557.0
61.00	2291.0
62.00	2208.0
63.00	1956.0
64.00	427.0
65.10	377.0
66.90	180.0
68.00	3866.0
69.00	3578.0
70.00	292.0
72.00	273.0
73.10	1808.0
74.00	6355.0
75.00	19632.0
76.00	1673.0
76.90	245.0
78.10	163.0
78.90	1846.0
80.00	541.0
80.90	1754.0
82.00	449.0
87.00	1316.0
87.90	1326.0
90.90	184.0
92.10	1174.0
93.00	1812.0
94.10	4973.0
95.10	35920.0
96.00	2252.0
97.00	134.0
103.90	312.0
105.90	239.0
108.10	131.0
112.90	102.0
116.00	201.0
116.90	319.0
118.00	204.0
119.00	243.0
127.70	125.0
129.90	219.0
135.00	115.0
136.90	136.0
140.90	521.0
142.90	633.0
144.90	249.0
147.90	139.0
158.90	102.0
171.00	105.0
171.90	606.0
174.00	27208.0
175.00	2307.0
176.00	27200.0
177.00	1735.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
35.10	120.0
36.00	376.0
37.00	2061.0
38.10	1748.0
39.10	817.0
40.00	203.0
40.80	106.0
44.10	756.0
45.00	347.0
47.00	455.0
48.10	333.0
49.00	1844.0
50.10	6981.0
51.00	2112.0
52.10	206.0
53.00	192.0
54.10	112.0
55.00	220.0
56.00	515.0
57.00	887.0
59.90	531.0
61.00	2184.0
62.00	2295.0
63.00	1793.0
64.00	408.0
65.10	362.0
66.90	144.0
68.00	3705.0
69.00	3662.0
70.00	258.0
72.00	282.0
73.00	1524.0
74.00	6382.0
75.10	19000.0
76.00	1662.0
76.90	265.0
77.80	162.0
78.20	166.0
78.90	1775.0
80.00	535.0
81.00	1678.0
81.90	427.0
87.00	1194.0
88.00	1293.0
90.90	163.0
92.00	1052.0
93.00	1696.0
94.10	4664.0
95.10	35736.0
96.10	2134.0
97.00	151.0
103.80	301.0
105.90	180.0
108.10	155.0
115.90	181.0
116.90	326.0
118.00	191.0
119.00	267.0
127.90	129.0
129.90	175.0
136.80	107.0
141.00	503.0
142.90	564.0
144.90	285.0
147.90	130.0
160.80	113.0
170.70	157.0
171.90	586.0
174.00	27568.0
175.00	2206.0
176.00	27416.0
177.00	1974.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

Scan 2790 (10.061 min): VV018719.D
BFB69

m/z	Abundance
39.50	137.0
40.10	200.0
44.10	490.0
47.80	115.0
53.20	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69