

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022665.D
 Acq On : 07 Oct 2021 15:53
 Operator : SY/MD
 Sample : VV1007WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK218

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	72	81	95	rBV	63994	65405	14.60%	1.870%
2	1.568	156	164	174	rBV	60478	67411	15.05%	1.927%
3	2.111	322	333	344	rBV	119469	164959	36.83%	4.716%
4	2.507	446	456	469	rVB	20180	32958	7.36%	0.942%
5	3.021	607	616	628	rVB6	6170	12311	2.75%	0.352%
6	3.995	895	919	955	rBV2	30094	159235	35.56%	4.552%
7	4.346	1008	1028	1051	rVB	78322	206012	46.00%	5.889%
8	5.044	1229	1245	1271	rBV3	201044	447837	100.00%	12.802%
9	5.619	1410	1424	1448	rBV	131087	262882	58.70%	7.515%
10	5.902	1496	1512	1525	rBV7	9031	18846	4.21%	0.539%
11	6.085	1553	1569	1589	rBV2	94809	202741	45.27%	5.796%
12	7.005	1845	1855	1878	rBV2	40986	76593	17.10%	2.190%
13	7.330	1942	1956	1976	rBV	192928	339490	75.81%	9.705%
14	7.638	2041	2052	2070	rBV2	25263	44927	10.03%	1.284%
15	8.114	2184	2200	2232	rBV3	174670	399912	89.30%	11.432%
16	8.860	2421	2432	2456	rBV	197435	320101	71.48%	9.151%
17	10.220	2842	2855	2869	rBV2	65281	101559	22.68%	2.903%
18	11.252	3165	3176	3190	rBV	184656	283069	63.21%	8.092%
19	11.625	3280	3292	3316	rVB	182759	291834	65.17%	8.343%




Sum of corrected areas: 3498082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022665.D
Acq On : 07 Oct 2021 15:53
Operator : SY/MD
Sample : VV1007WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

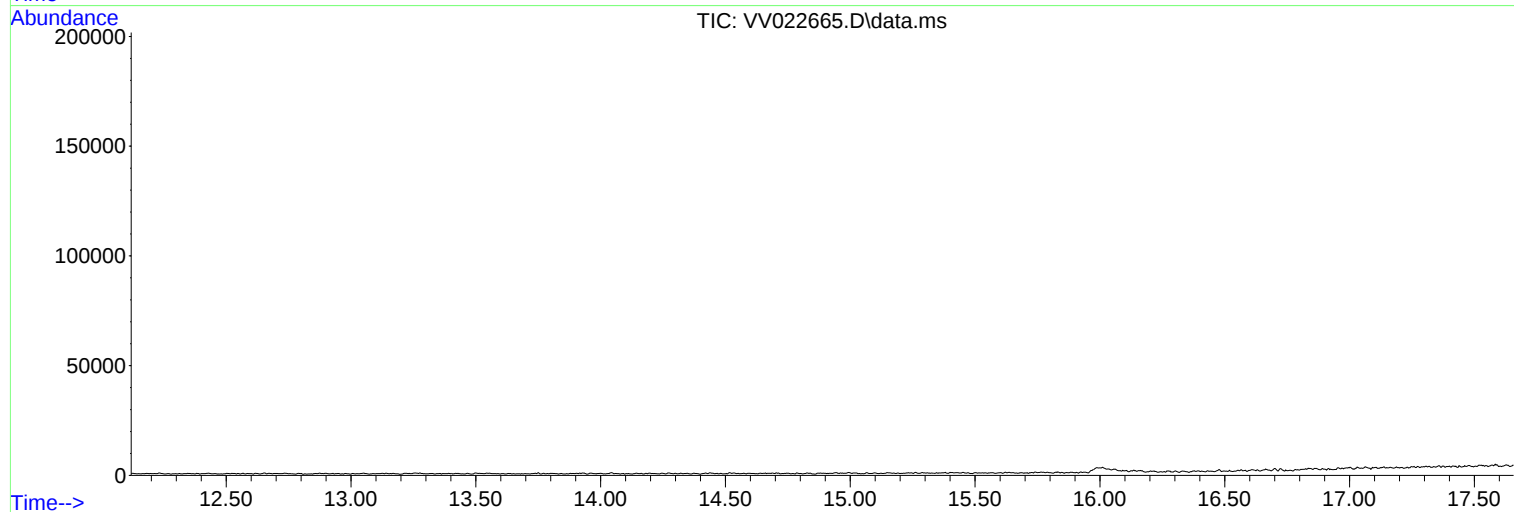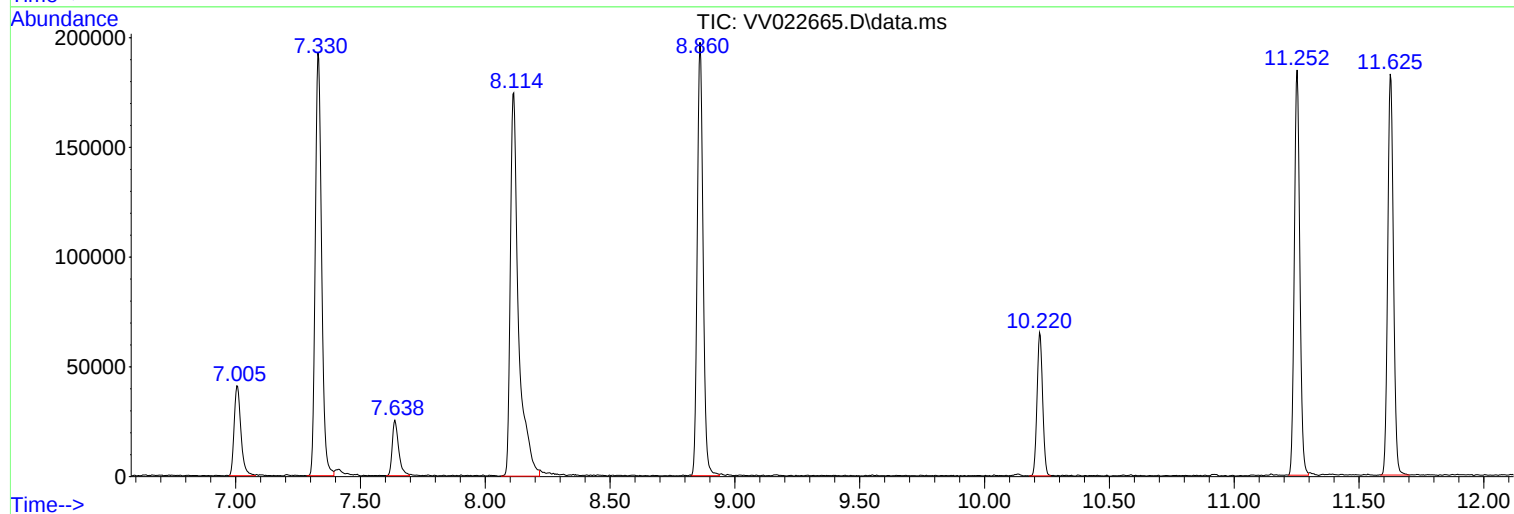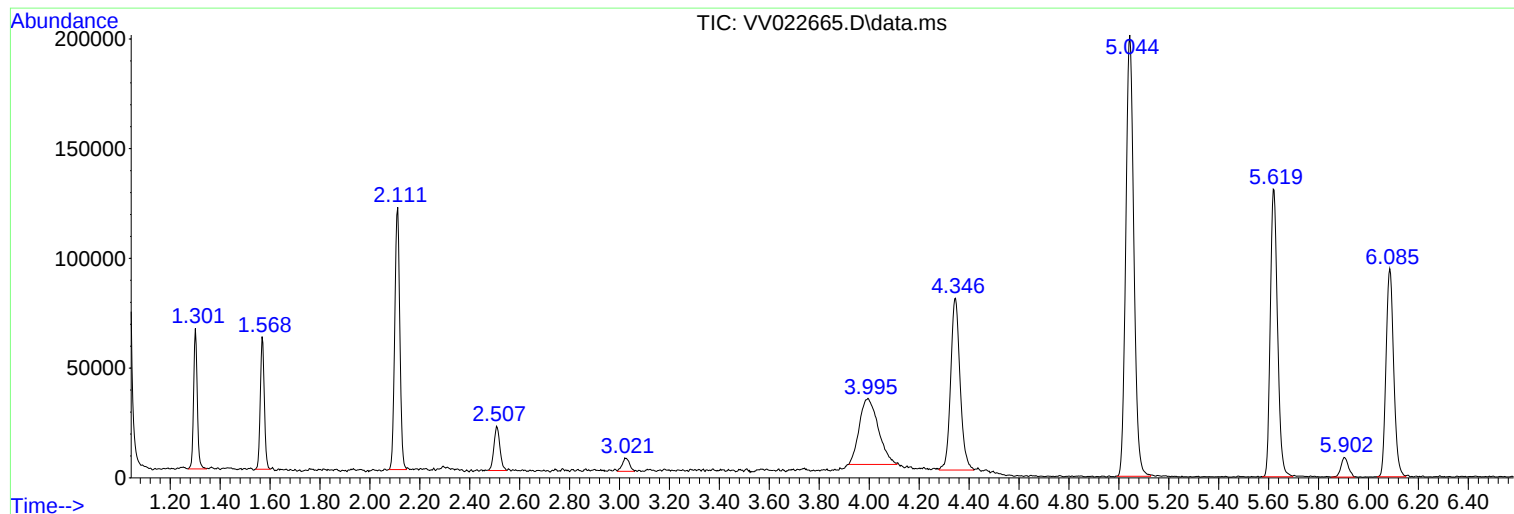

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022665.D
Acq On : 07 Oct 2021 15:53
Operator : SY/MD
Sample : VV1007WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022665.D
Acq On : 07 Oct 2021 15:53
Operator : SY/MD
Sample : VV1007WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
