

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022667.D
 Acq On : 07 Oct 2021 17:05
 Operator : SY/MD
 Sample : M4050-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	38	rVB	7227	7287	1.76%	0.203%
2	1.304	71	82	92	rBV2	70152	86702	20.89%	2.409%
3	1.568	156	164	173	rBV	62819	72575	17.49%	2.017%
4	2.108	320	332	345	rBV	119075	173058	41.70%	4.809%
5	2.182	345	355	368	rVV2	4510	10624	2.56%	0.295%
6	3.895	877	888	925	rBV2	39910	155409	37.45%	4.319%
7	4.349	1011	1029	1052	rBV	73905	184241	44.40%	5.120%
8	5.050	1231	1247	1272	rBV2	165145	414998	100.00%	11.533%
9	5.619	1412	1424	1445	rBV2	130251	267184	64.38%	7.425%
10	5.908	1504	1514	1528	rVB2	11411	22611	5.45%	0.628%
11	6.072	1552	1565	1589	rBV	94203	196708	47.40%	5.467%
12	6.587	1712	1725	1736	rBV4	2974	6198	1.49%	0.172%
13	6.989	1836	1850	1868	rBV	41151	75431	18.18%	2.096%
14	7.317	1940	1952	1968	rBV	194499	341239	82.23%	9.483%
15	7.394	1968	1976	1988	rVB2	12329	22292	5.37%	0.619%
16	7.625	2039	2048	2068	rBV	24764	44920	10.82%	1.248%
17	7.982	2149	2159	2169	rVB4	12103	20337	4.90%	0.565%
18	8.095	2182	2194	2227	rBV2	166721	387990	93.49%	10.782%
19	8.853	2419	2430	2449	rBV	204876	339946	81.92%	9.447%
20	8.969	2458	2466	2474	rVB6	3140	5109	1.23%	0.142%
21	9.021	2474	2482	2492	rBV4	2983	4773	1.15%	0.133%
22	9.140	2509	2519	2535	rBV2	14142	24078	5.80%	0.669%
23	9.551	2637	2647	2662	rBV5	8865	17559	4.23%	0.488%
24	10.217	2843	2854	2869	rBV	57709	91485	22.04%	2.542%
25	11.249	3163	3175	3194	rBV	197599	311310	75.01%	8.651%
26	11.532	3255	3263	3274	rBV4	5182	8428	2.03%	0.234%
27	11.625	3281	3292	3309	rBV	193740	305930	73.72%	8.502%




Sum of corrected areas: 3598422

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022667.D
Acq On : 07 Oct 2021 17:05
Operator : SY/MD
Sample : M4050-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

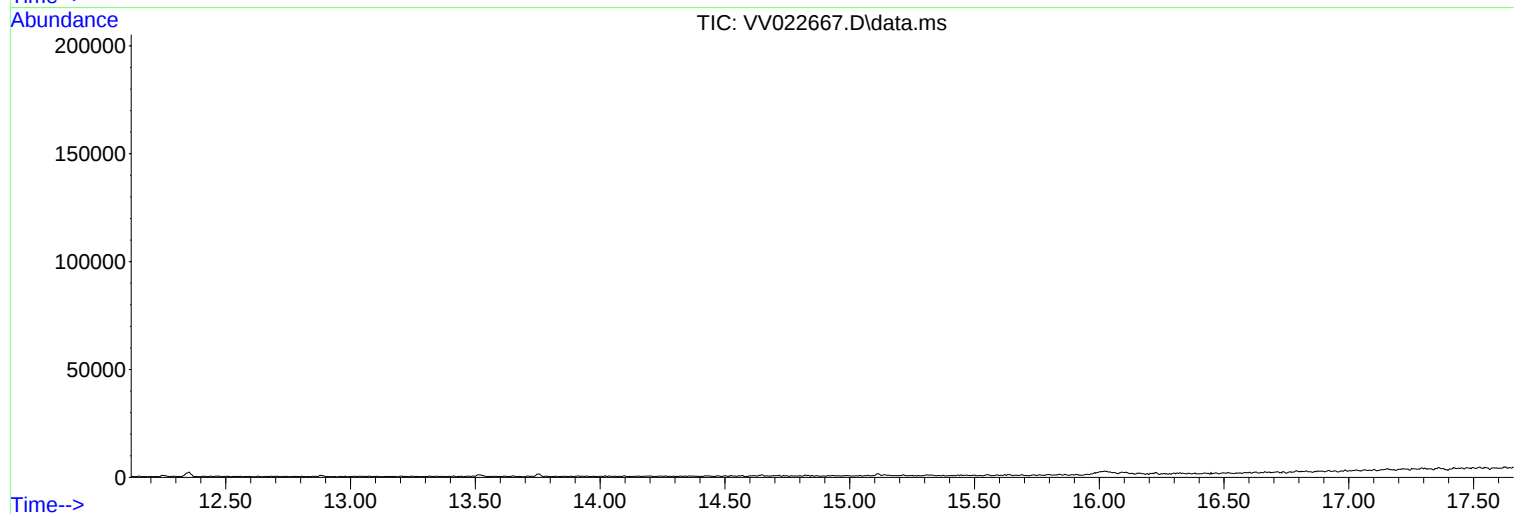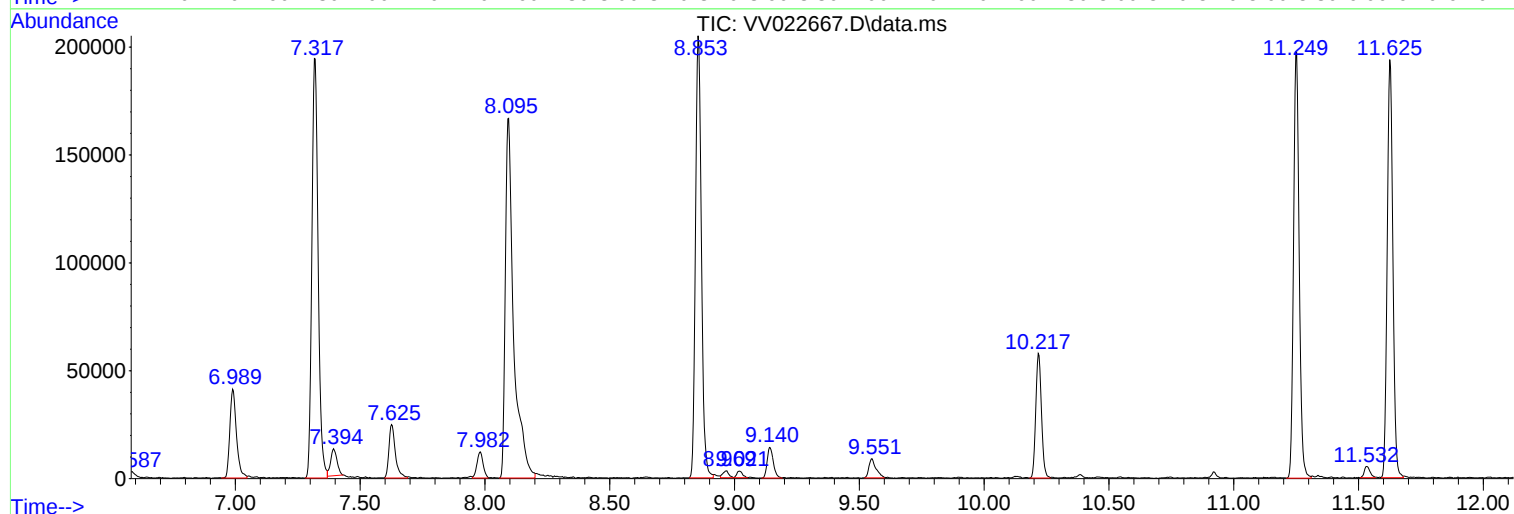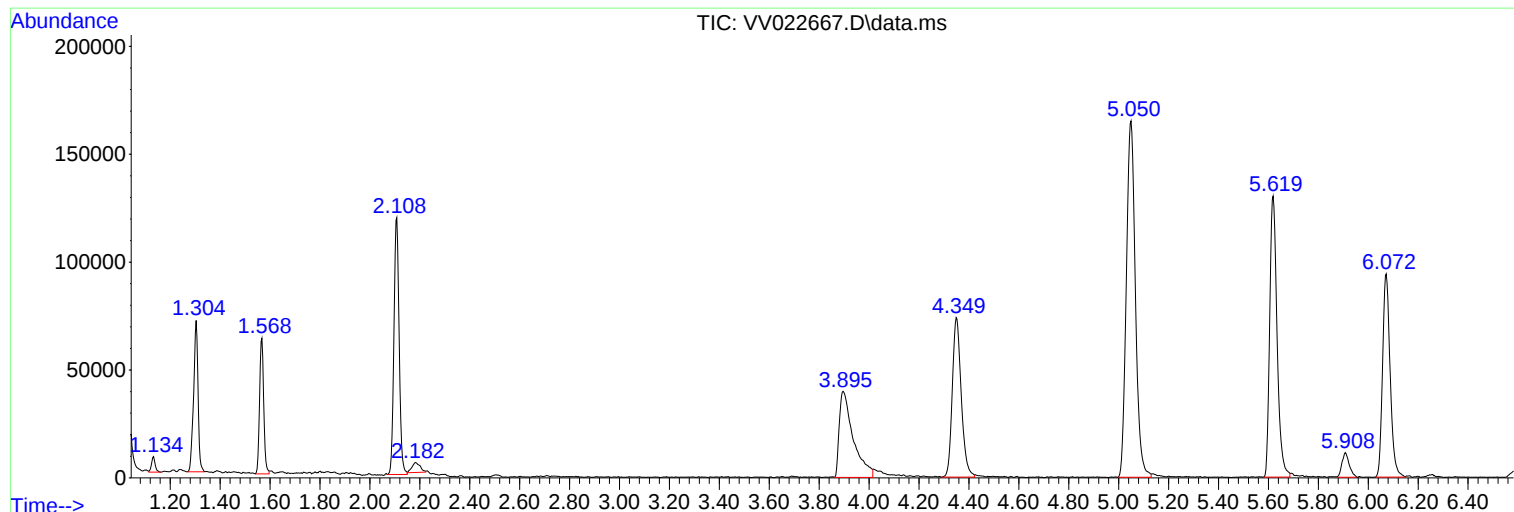

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022667.D
Acq On : 07 Oct 2021 17:05
Operator : SY/MD
Sample : M4050-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022667.D
Acq On : 07 Oct 2021 17:05
Operator : SY/MD
Sample : M4050-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
