

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022671.D
 Acq On : 07 Oct 2021 18:41
 Operator : SY/MD
 Sample : M4051-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	61393	61221	15.31%	1.780%
2	1.568	155	164	173	rBV	60631	68612	17.16%	1.995%
3	2.105	319	331	345	rBV	110974	161091	40.30%	4.684%
4	3.912	876	893	924	rBV	35328	124730	31.20%	3.627%
5	4.352	1013	1030	1058	rVB2	55621	185435	46.39%	5.392%
6	4.825	1163	1177	1191	rBV4	4186	10196	2.55%	0.296%
7	5.047	1230	1246	1271	rBV2	167273	399772	100.00%	11.624%
8	5.619	1412	1424	1451	rBV	131093	265232	66.35%	7.712%
9	5.915	1503	1516	1535	rBV3	31061	68346	17.10%	1.987%
10	6.072	1551	1565	1586	rBV	94080	192291	48.10%	5.591%
11	6.989	1840	1850	1867	rBV2	38361	70719	17.69%	2.056%
12	7.317	1941	1952	1967	rBV	181544	313981	78.54%	9.130%
13	7.397	1972	1977	1991	rVB2	5849	10145	2.54%	0.295%
14	7.625	2037	2048	2063	rBV2	22643	40887	10.23%	1.189%
15	7.976	2147	2157	2173	rVB	34739	59095	14.78%	1.718%
16	8.098	2183	2195	2238	rBV2	150209	393328	98.39%	11.437%
17	8.854	2419	2430	2458	rBV	203309	335559	83.94%	9.757%
18	10.220	2844	2855	2869	rBV	63829	102210	25.57%	2.972%
19	11.249	3163	3175	3196	rBV	181970	288601	72.19%	8.392%
20	11.625	3280	3292	3309	rBV	179684	287656	71.96%	8.364%




Sum of corrected areas: 3439107

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022671.D
Acq On : 07 Oct 2021 18:41
Operator : SY/MD
Sample : M4051-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

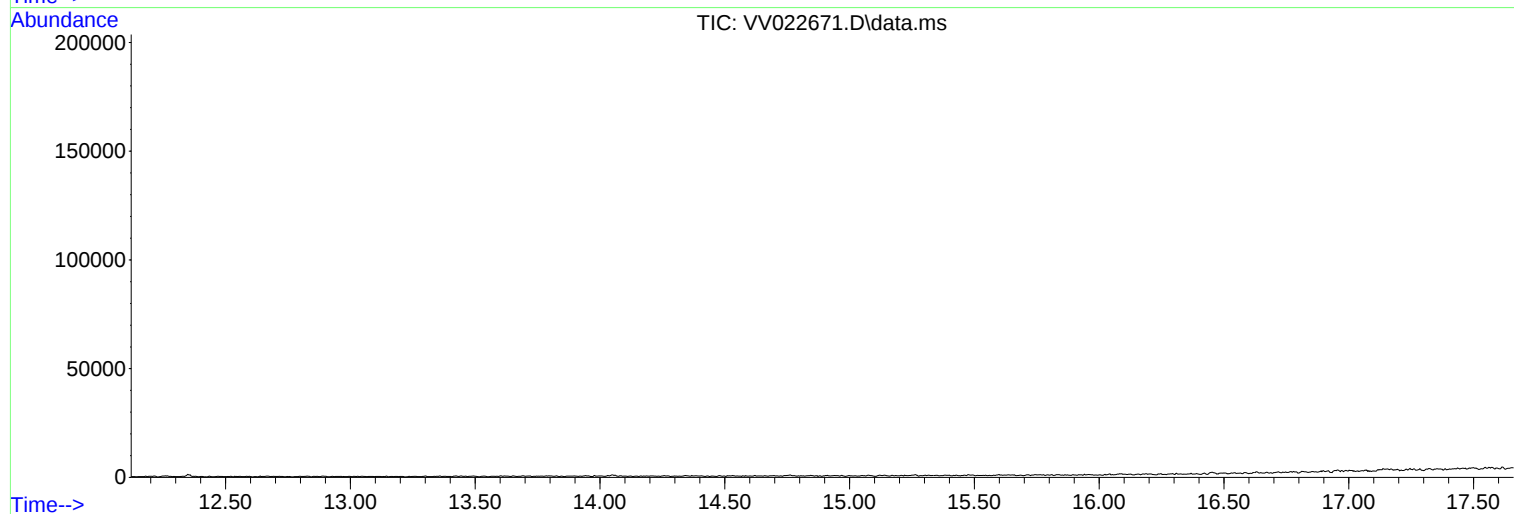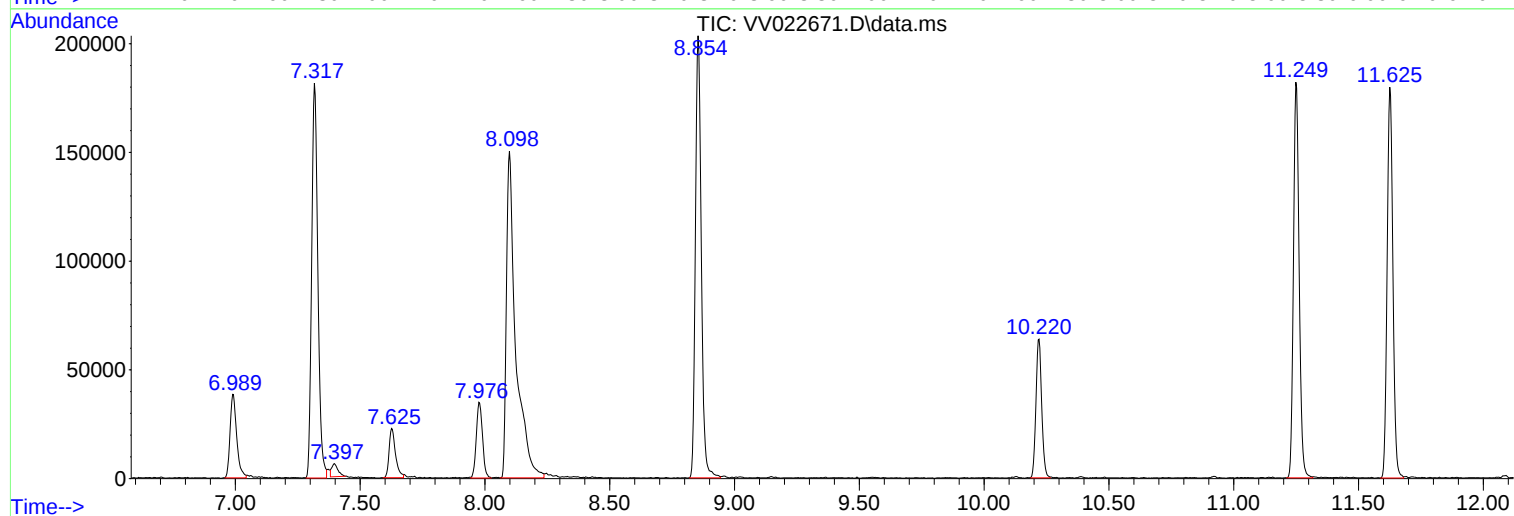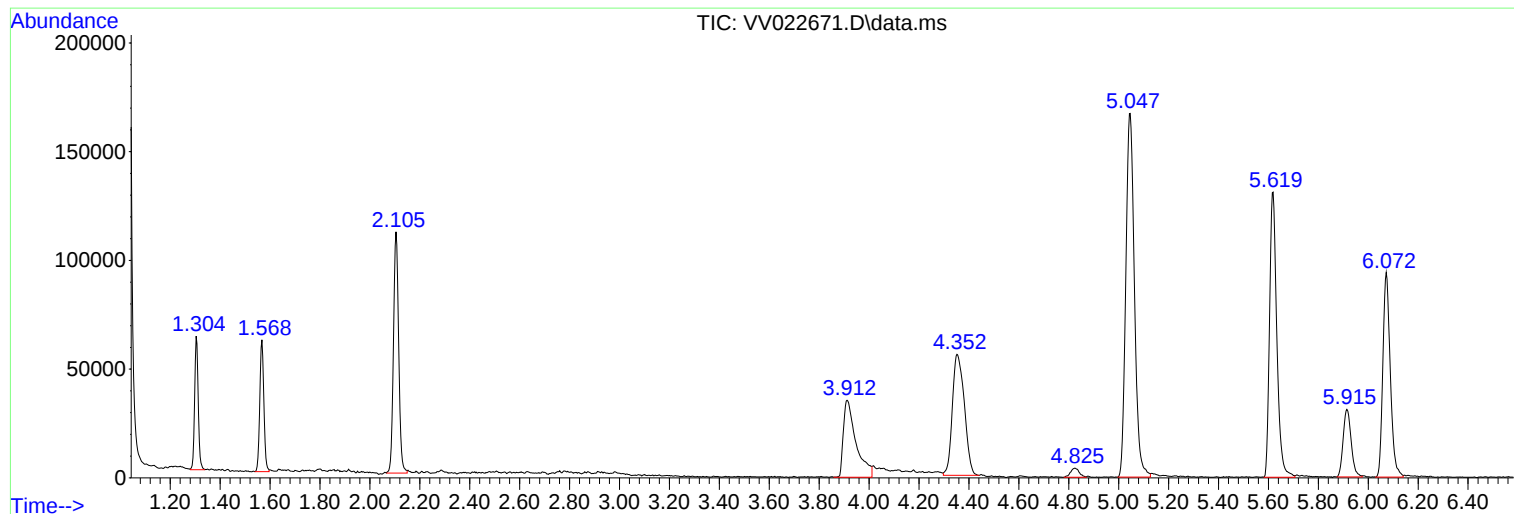

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022671.D
Acq On : 07 Oct 2021 18:41
Operator : SY/MD
Sample : M4051-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022671.D
Acq On : 07 Oct 2021 18:41
Operator : SY/MD
Sample : M4051-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
