

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022675.D
 Acq On : 07 Oct 2021 20:17
 Operator : SY/MD
 Sample : M4052-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	62891	61784	15.29%	1.731%
2	1.564	156	163	172	rBV	57270	64285	15.91%	1.801%
3	1.751	216	221	229	rVB3	4680	5462	1.35%	0.153%
4	2.105	320	331	346	rBV2	110778	163275	40.41%	4.575%
5	3.915	882	894	935	rBV	29154	136377	33.75%	3.821%
6	4.352	1012	1030	1060	rVB3	56456	183512	45.42%	5.142%
7	4.825	1164	1177	1196	rVB3	2931	7121	1.76%	0.200%
8	5.047	1230	1246	1274	rBV2	166802	404060	100.00%	11.322%
9	5.619	1412	1424	1443	rBV	120383	245440	60.74%	6.878%
10	5.915	1503	1516	1537	rBV6	29826	66140	16.37%	1.853%
11	6.072	1551	1565	1589	rBV	92987	196159	48.55%	5.497%
12	6.989	1840	1850	1874	rBV	38471	73148	18.10%	2.050%
13	7.317	1940	1952	1969	rBV	181171	317637	78.61%	8.901%
14	7.397	1970	1977	1994	rVB	8169	16066	3.98%	0.450%
15	7.625	2039	2048	2064	rBV	22600	40719	10.08%	1.141%
16	7.976	2141	2157	2174	rBV	124538	213231	52.77%	5.975%
17	8.098	2183	2195	2234	rBV3	154712	393536	97.40%	11.027%
18	8.853	2419	2430	2453	rBV	186039	310967	76.96%	8.714%
19	10.220	2843	2855	2873	rBV	65445	103772	25.68%	2.908%
20	11.249	3161	3175	3195	rBV	180301	278892	69.02%	7.815%
21	11.625	3279	3292	3310	rBV	181582	287129	71.06%	8.046%




Sum of corrected areas: 3568712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022675.D
Acq On : 07 Oct 2021 20:17
Operator : SY/MD
Sample : M4052-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

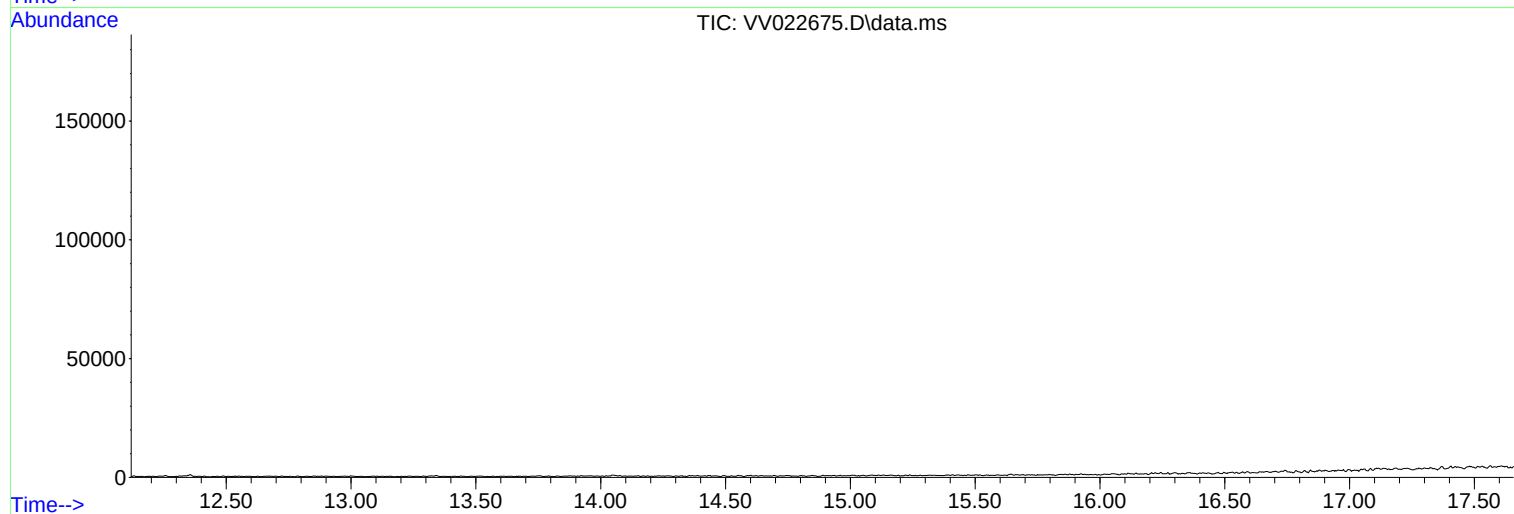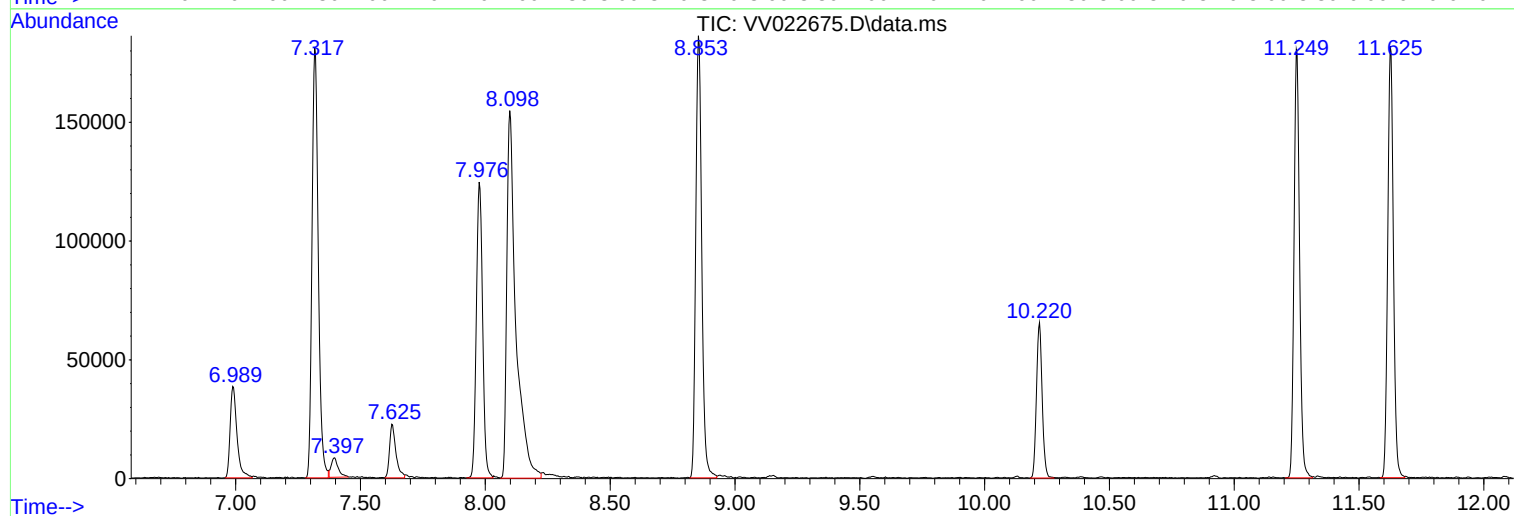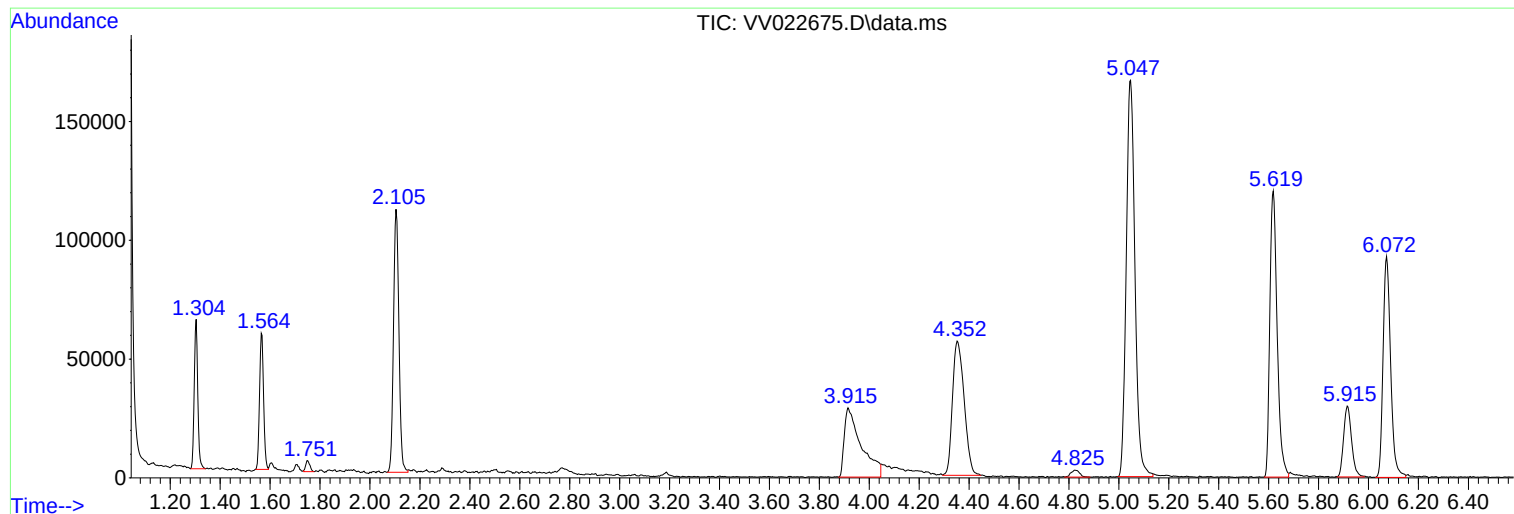

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022675.D
Acq On : 07 Oct 2021 20:17
Operator : SY/MD
Sample : M4052-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022675.D
Acq On : 07 Oct 2021 20:17
Operator : SY/MD
Sample : M4052-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
