

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022678.D
 Acq On : 07 Oct 2021 21:29
 Operator : SY/MD
 Sample : M4052-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rBV	57074	57108	9.51%	1.286%
2	1.568	156	164	174	rBV	54622	62696	10.44%	1.411%
3	2.111	321	333	348	rBV3	157718	267714	44.58%	6.026%
4	3.191	656	669	680	rBV3	3131	6414	1.07%	0.144%
5	3.912	880	893	916	rBV3	62517	193553	32.23%	4.357%
6	4.352	1013	1030	1062	rVB4	54520	169340	28.20%	3.812%
7	4.609	1098	1110	1124	rBV3	3690	8838	1.47%	0.199%
8	5.050	1231	1247	1278	rBV2	146986	370588	61.71%	8.342%
9	5.619	1409	1424	1453	rBV	120168	253776	42.26%	5.713%
10	5.915	1503	1516	1547	rBV	278639	551465	91.84%	12.414%
11	6.072	1552	1565	1589	rVB	85182	177000	29.48%	3.984%
12	6.989	1840	1850	1873	rBV	35282	67129	11.18%	1.511%
13	7.317	1941	1952	1969	rBV	168048	297264	49.50%	6.691%
14	7.625	2040	2048	2066	rBV2	20541	37626	6.27%	0.847%
15	7.976	2145	2157	2181	rBV	358944	600485	100.00%	13.517%
16	8.095	2183	2194	2225	rBV2	144366	360368	60.01%	8.112%
17	8.853	2419	2430	2453	rBV	192766	319267	53.17%	7.187%
18	10.220	2844	2855	2869	rBV2	59923	94260	15.70%	2.122%
19	11.249	3164	3175	3197	rBV	178437	283435	47.20%	6.380%
20	11.625	3280	3292	3309	rBV	165443	264126	43.99%	5.946%




Sum of corrected areas: 4442452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022678.D
Acq On : 07 Oct 2021 21:29
Operator : SY/MD
Sample : M4052-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

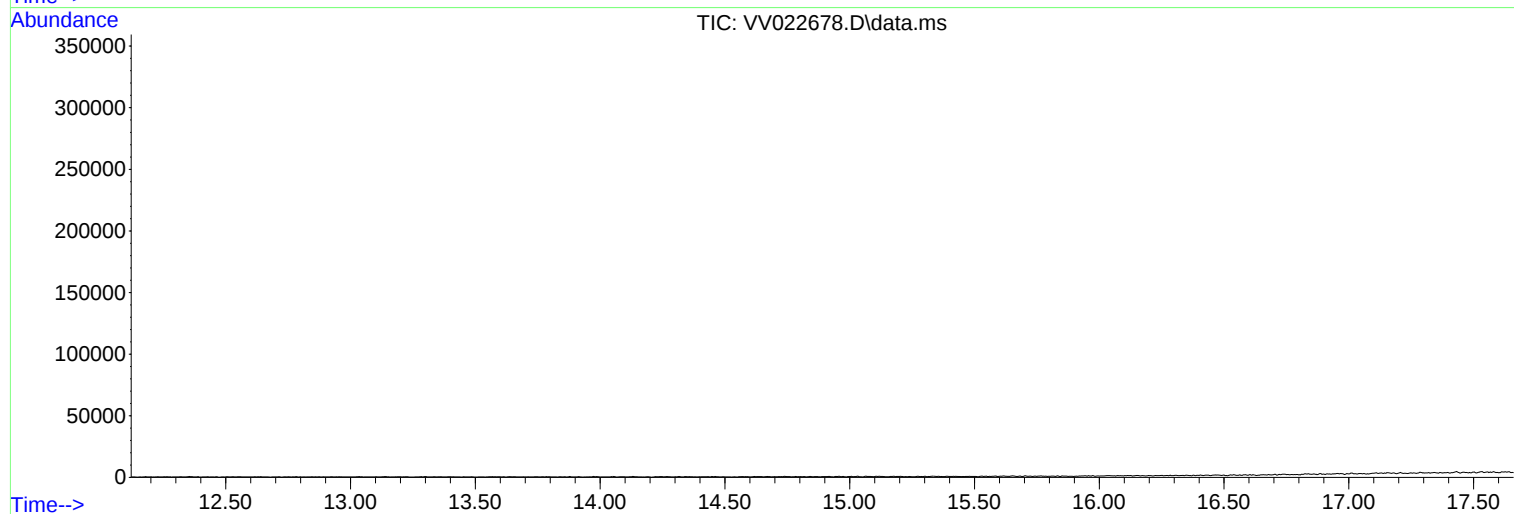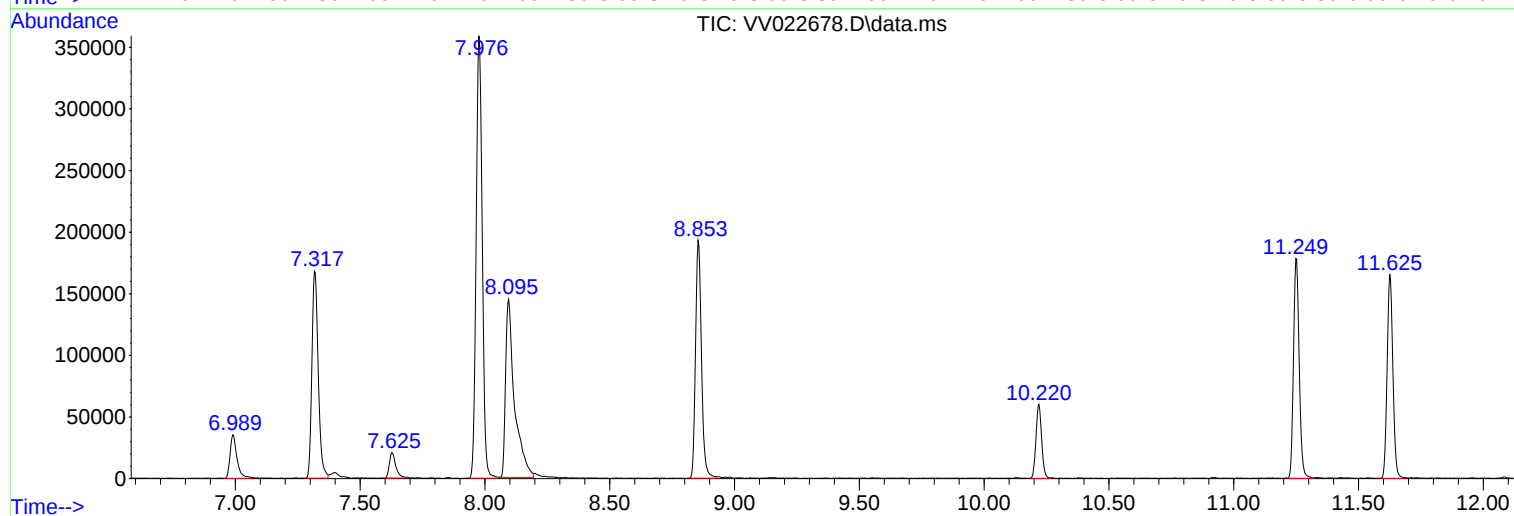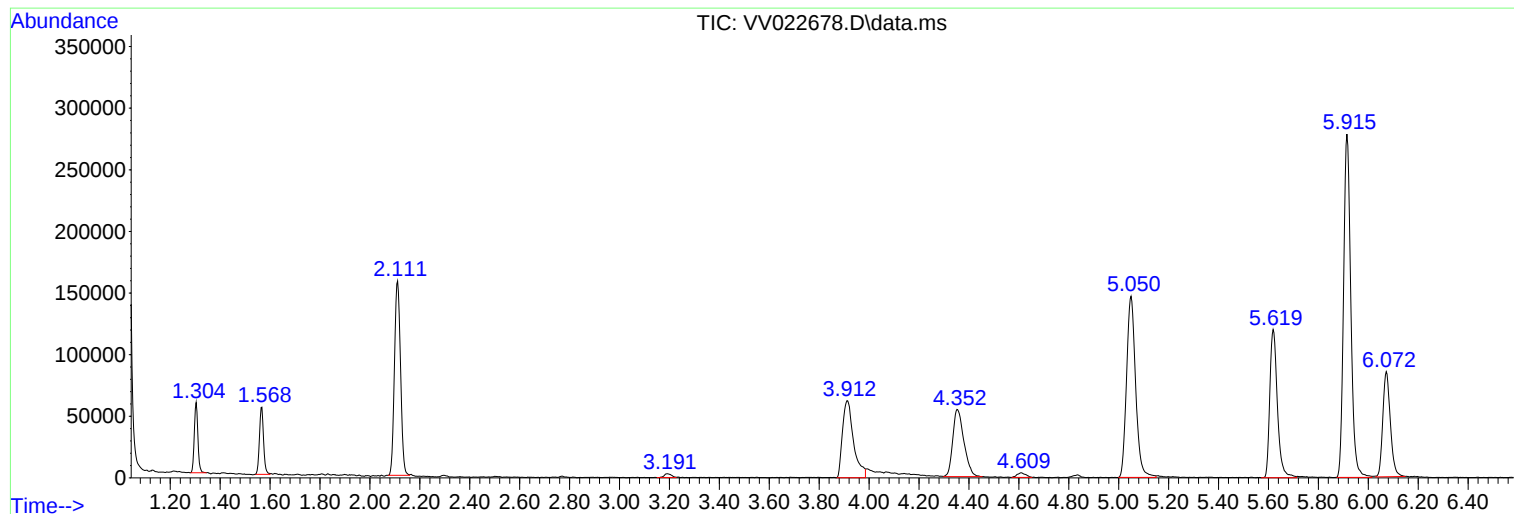

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022678.D
Acq On : 07 Oct 2021 21:29
Operator : SY/MD
Sample : M4052-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022678.D
Acq On : 07 Oct 2021 21:29
Operator : SY/MD
Sample : M4052-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
