

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022680.D
 Acq On : 07 Oct 2021 22:16
 Operator : SY/MD
 Sample : M4052-06DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	43	50	69	rVB	184542	168305	28.07%	4.296%
2	1.304	75	82	94	rVB	61783	60710	10.13%	1.550%
3	1.564	156	163	177	rBV	57247	65604	10.94%	1.675%
4	2.105	321	331	348	rBV	104606	154013	25.69%	3.931%
5	2.507	447	456	469	rVB2	9354	15889	2.65%	0.406%
6	3.908	880	892	916	rBV	31996	123677	20.63%	3.157%
7	4.352	1012	1030	1059	rBV3	60192	172563	28.78%	4.405%
8	5.050	1230	1247	1273	rBV2	152133	382364	63.77%	9.760%
9	5.619	1412	1424	1449	rBV	120194	246744	41.15%	6.298%
10	5.915	1504	1516	1528	rVB9	7261	15265	2.55%	0.390%
11	6.072	1549	1565	1585	rBV	88470	183476	30.60%	4.683%
12	6.992	1838	1851	1869	rBV2	36025	68027	11.35%	1.736%
13	7.317	1940	1952	1972	rBV	170861	301808	50.34%	7.704%
14	7.397	1972	1977	1990	rVB2	3840	7319	1.22%	0.187%
15	7.625	2037	2048	2065	rBV	22170	39206	6.54%	1.001%
16	7.976	2141	2157	2179	rBV	357965	599562	100.00%	15.304%
17	8.095	2183	2194	2230	rBV2	171173	364248	60.75%	9.298%
18	8.854	2419	2430	2451	rBV	189836	310697	51.82%	7.931%
19	10.217	2843	2854	2868	rBV2	59697	95511	15.93%	2.438%
20	11.252	3164	3176	3197	rBV	173273	273199	45.57%	6.974%
21	11.625	3280	3292	3310	rBV	169802	269440	44.94%	6.878%




Sum of corrected areas: 3917627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022680.D
Acq On : 07 Oct 2021 22:16
Operator : SY/MD
Sample : M4052-06DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

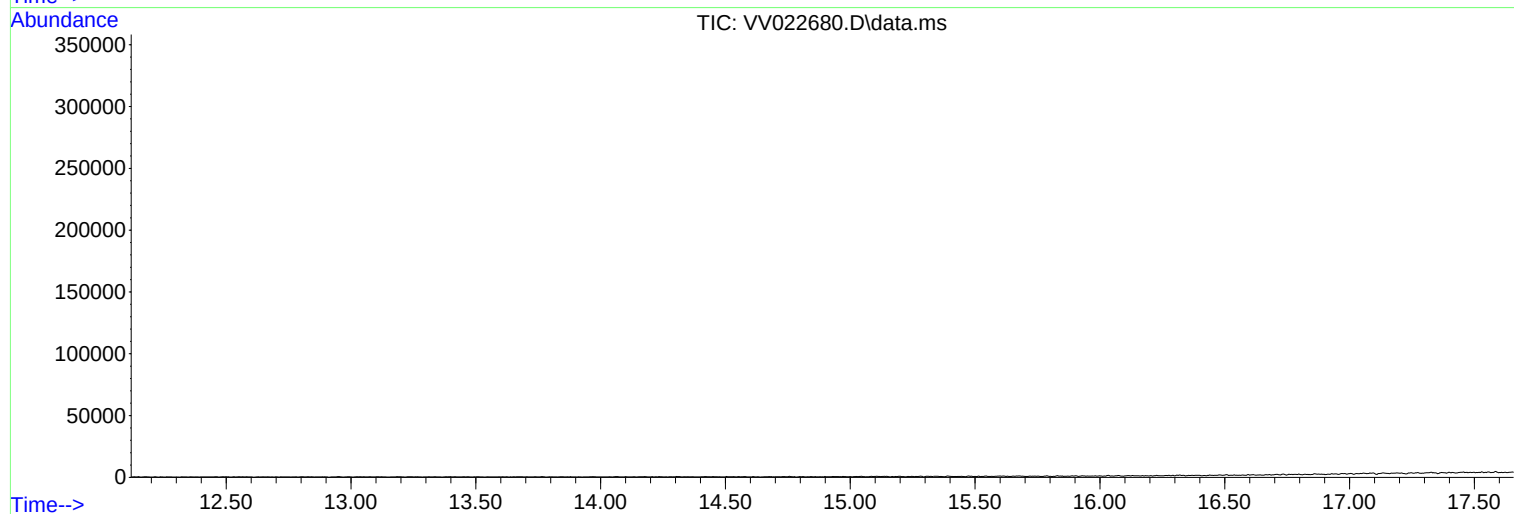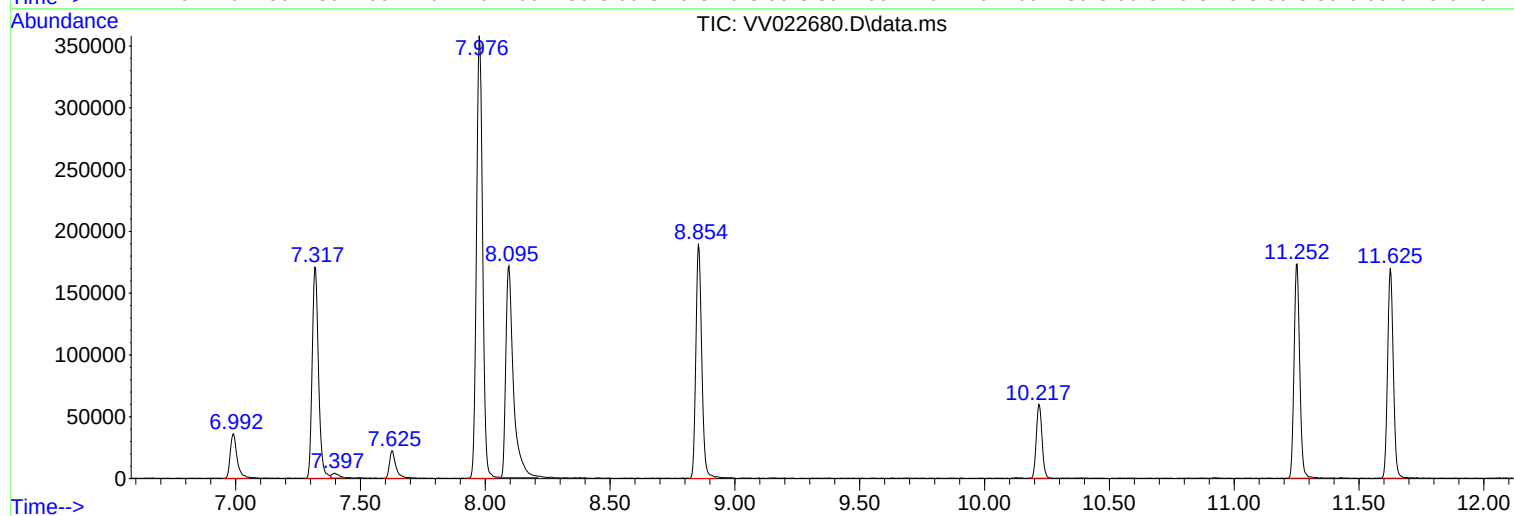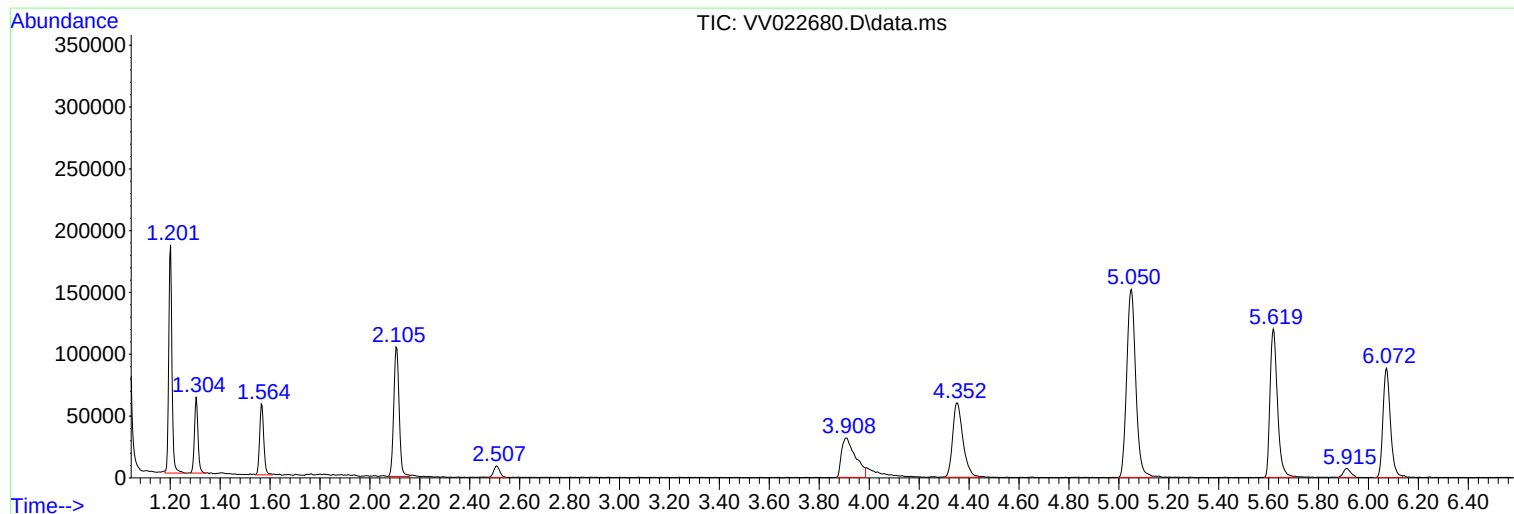

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022680.D
Acq On : 07 Oct 2021 22:16
Operator : SY/MD
Sample : M4052-06DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX6DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	3.41 ug/L	168305	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			Ethyne, chloro-	60	C2HCl	000593-63-5	5
3			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
4			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4
5			Cyanogen chloride	61	CClN	000506-77-4	4

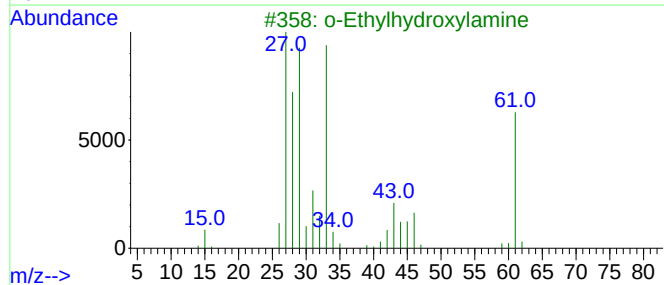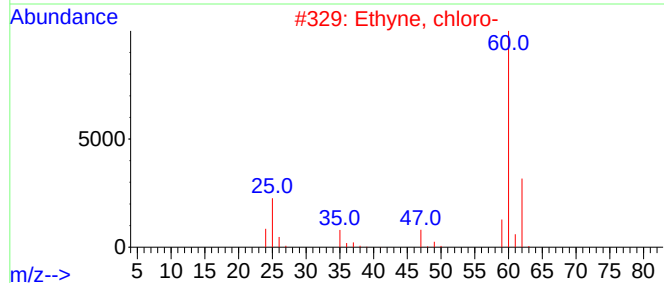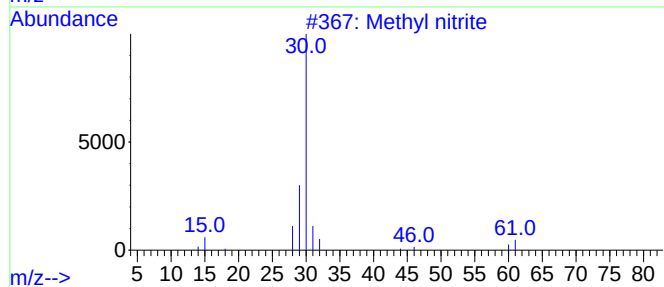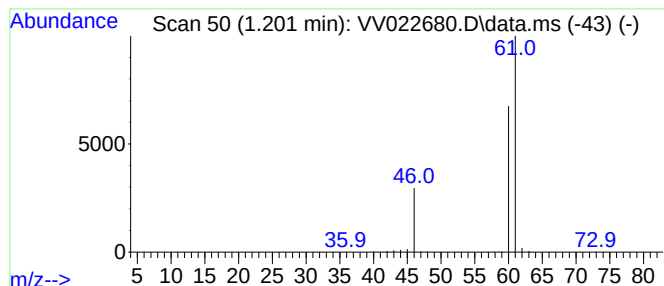

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022680.D
Acq On : 07 Oct 2021 22:16
Operator : SY/MD
Sample : M4052-06DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	3.4	ug/L	168305	1	5.619	246744	5.0