

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022682.D
 Acq On : 07 Oct 2021 23:04
 Operator : SY/MD
 Sample : M4052-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	63337	67041	3.74%	0.963%
2	1.568	156	164	178	rBV	59367	68319	3.81%	0.981%
3	2.114	319	334	353	rBV5	350329	572280	31.91%	8.217%
4	3.192	655	669	687	rBV	15600	34121	1.90%	0.490%
5	3.912	876	893	938	rBV2	224612	632785	35.29%	9.086%
6	4.355	1014	1031	1058	rBV5	55273	187234	10.44%	2.688%
7	4.609	1096	1110	1126	rVB3	8106	19203	1.07%	0.276%
8	5.050	1231	1247	1280	rBV2	162450	409651	22.84%	5.882%
9	5.619	1412	1424	1454	rBV	121569	247765	13.82%	3.558%
10	5.915	1503	1516	1545	rBV	457848	899170	50.14%	12.911%
11	6.072	1552	1565	1583	rBV	94066	191650	10.69%	2.752%
12	6.989	1840	1850	1868	rBV2	38392	72263	4.03%	1.038%
13	7.317	1938	1952	1970	rBV	184485	328495	18.32%	4.717%
14	7.625	2039	2048	2066	rBV	23226	41364	2.31%	0.594%
15	7.976	2143	2157	2179	rBV	1073777	1793228	100.00%	25.748%
16	8.092	2183	2193	2237	rVB2	191948	406486	22.67%	5.837%
17	8.854	2419	2430	2455	rBV	191138	315117	17.57%	4.525%
18	10.217	2841	2854	2873	rBV2	65550	104316	5.82%	1.498%
19	11.249	3162	3175	3193	rBV	180129	281307	15.69%	4.039%
20	11.625	3280	3292	3308	rBV	183587	292636	16.32%	4.202%




Sum of corrected areas: 6964431

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022682.D
Acq On : 07 Oct 2021 23:04
Operator : SY/MD
Sample : M4052-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

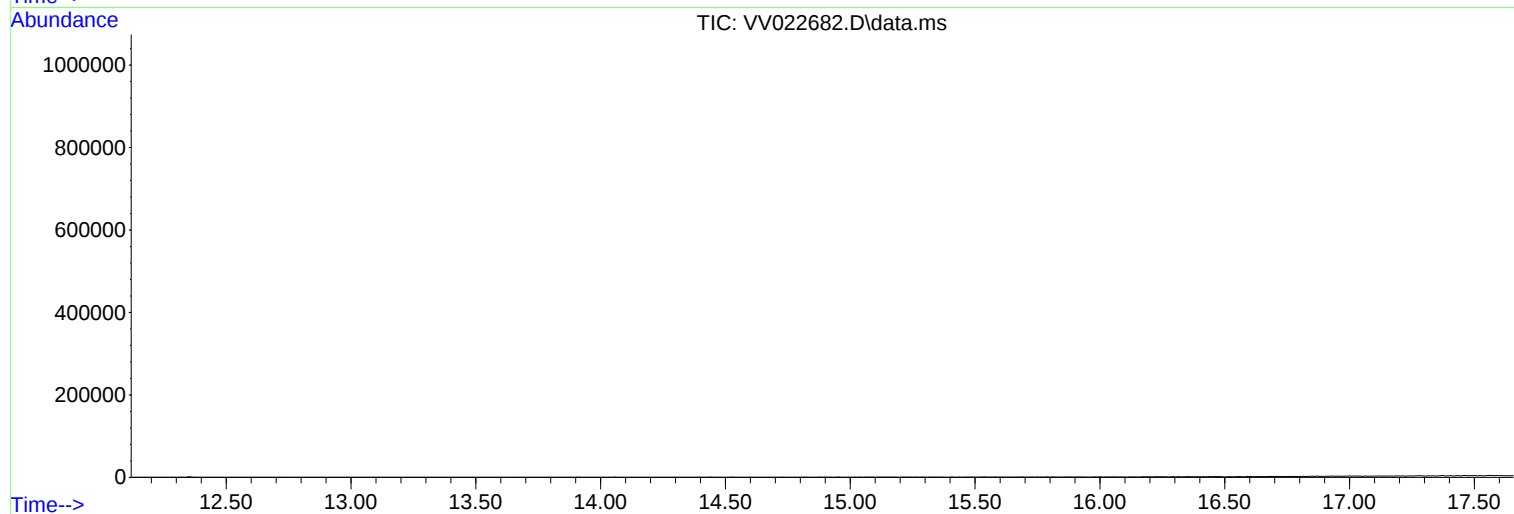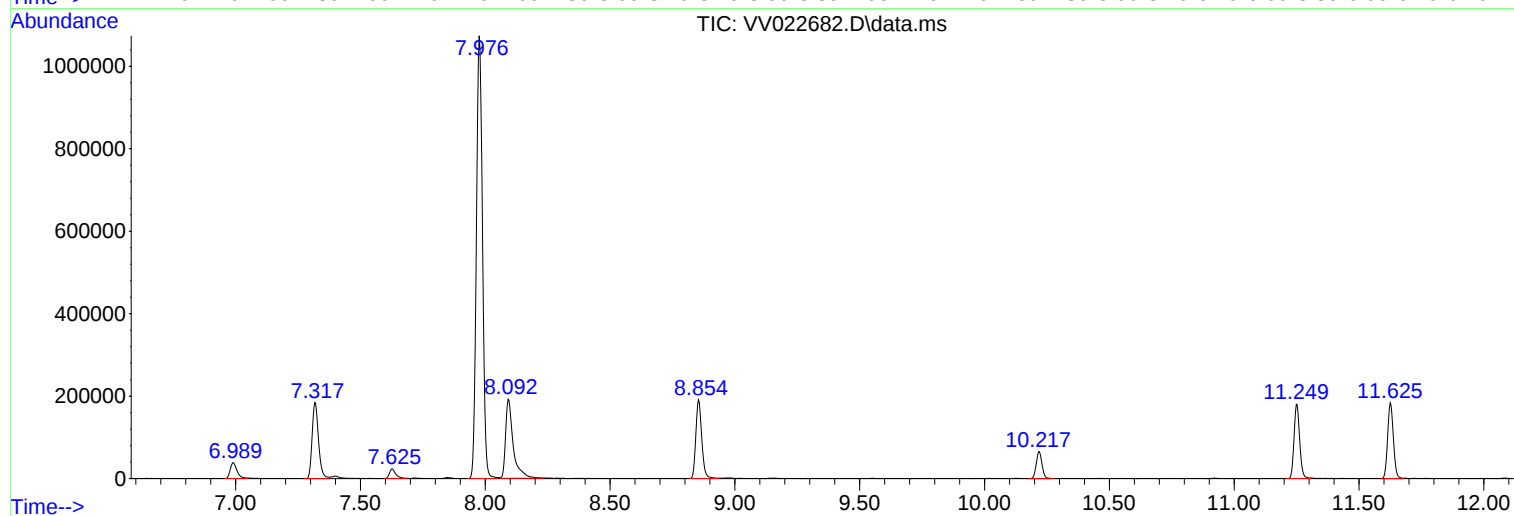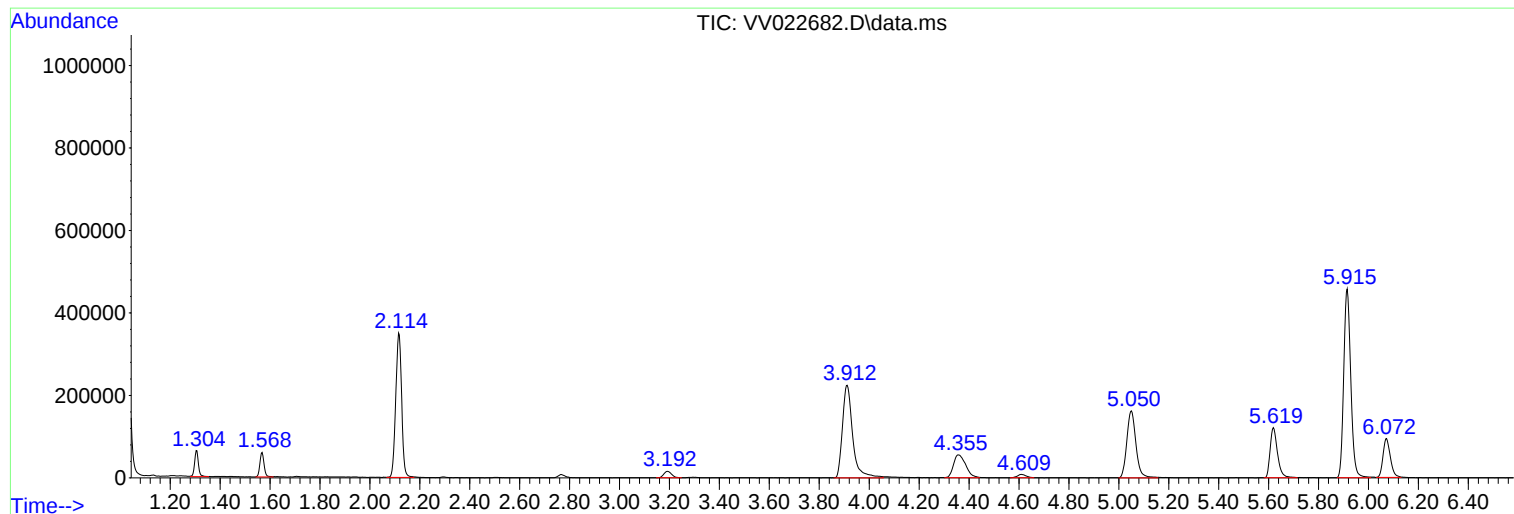

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022682.D
Acq On : 07 Oct 2021 23:04
Operator : SY/MD
Sample : M4052-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022682.D
Acq On : 07 Oct 2021 23:04
Operator : SY/MD
Sample : M4052-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
