

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022687.D
 Acq On : 08 Oct 2021 01:04
 Operator : SY/MD
 Sample : M4098-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT37

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	61072	63201	15.23%	1.820%
2	1.568	156	164	173	rBV	61496	68874	16.60%	1.983%
3	2.108	321	332	347	rVB	113281	162478	39.16%	4.679%
4	3.899	878	889	937	rBV	41850	169906	40.95%	4.893%
5	4.352	1014	1030	1056	rBV	67668	181693	43.79%	5.232%
6	5.050	1227	1247	1276	rBV2	165615	414929	100.00%	11.949%
7	5.619	1412	1424	1448	rBV	128981	264285	63.69%	7.611%
8	5.911	1505	1515	1534	rVB8	5011	10842	2.61%	0.312%
9	6.072	1552	1565	1589	rBV2	96203	198545	47.85%	5.718%
10	6.989	1838	1850	1866	rBV2	39083	73071	17.61%	2.104%
11	7.317	1940	1952	1972	rBV	188628	333519	80.38%	9.605%
12	7.397	1972	1977	1992	rVB7	2678	5278	1.27%	0.152%
13	7.625	2039	2048	2068	rBV	22634	42387	10.22%	1.221%
14	8.091	2183	2193	2229	rBV2	188183	409263	98.63%	11.786%
15	8.853	2419	2430	2453	rBV	198532	331627	79.92%	9.550%
16	10.217	2842	2854	2871	rBV2	68342	108918	26.25%	3.137%
17	11.249	3164	3175	3198	rBV	191315	302891	73.00%	8.723%
18	11.532	3257	3263	3277	rVB5	5065	7890	1.90%	0.227%
19	11.625	3277	3292	3312	rBV	195896	308268	74.29%	8.878%
20	13.056	3726	3737	3747	rVB3	3815	6168	1.49%	0.178%
21	13.506	3866	3877	3887	rBV5	3385	8377	2.02%	0.241%




Sum of corrected areas: 3472410

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022687.D
Acq On : 08 Oct 2021 01:04
Operator : SY/MD
Sample : M4098-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

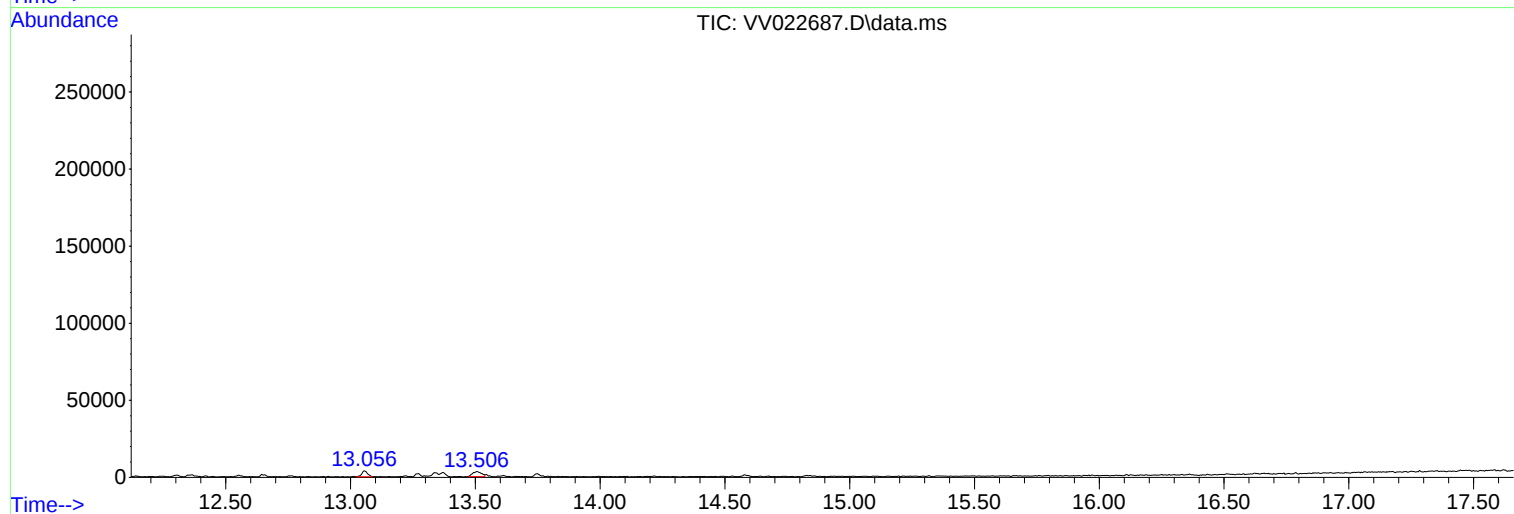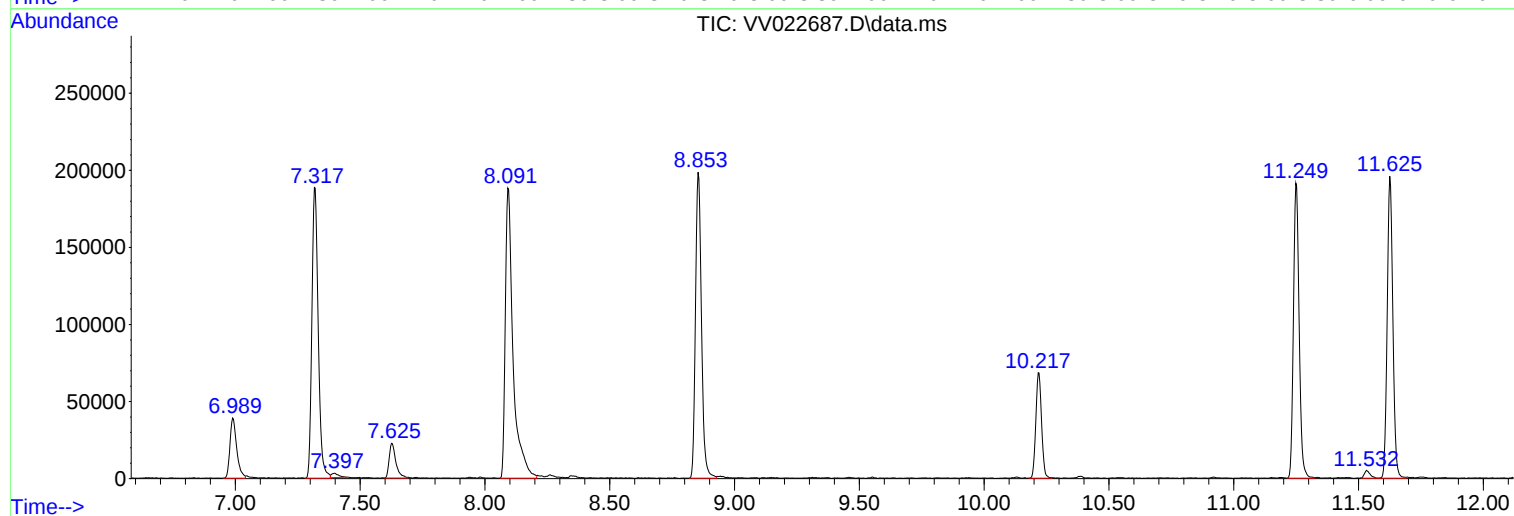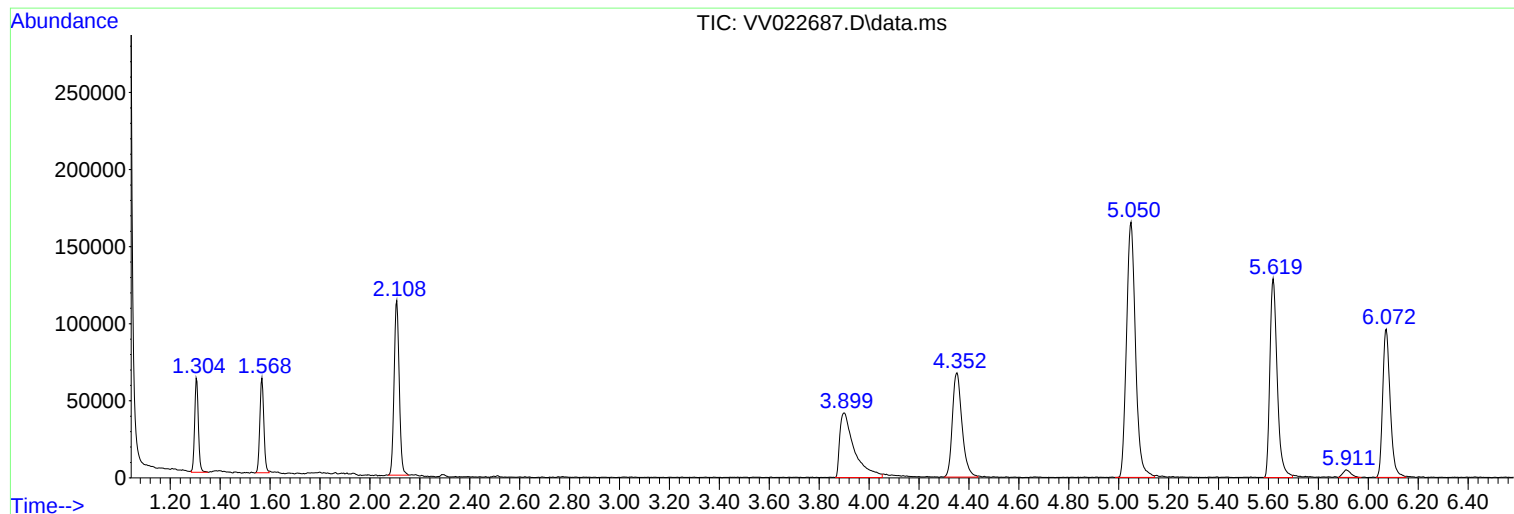

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022687.D
Acq On : 08 Oct 2021 01:04
Operator : SY/MD
Sample : M4098-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
Data File : VV022687.D
Acq On : 08 Oct 2021 01:04
Operator : SY/MD
Sample : M4098-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
