
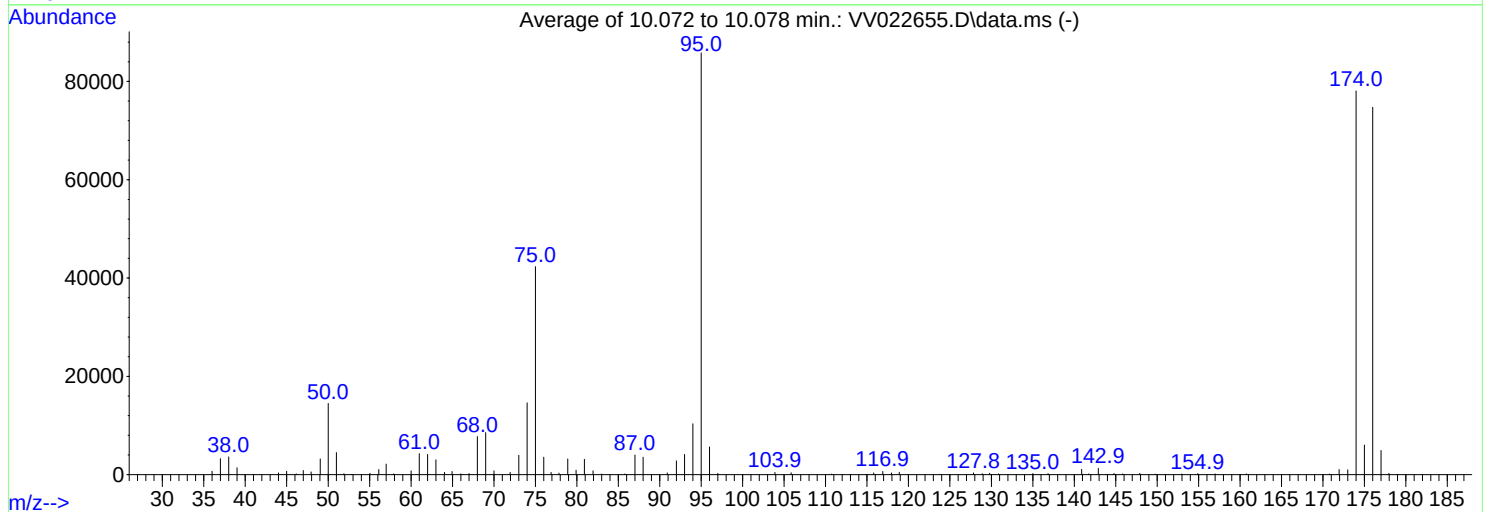


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100721\
 Data File : VV022655.D
 Acq On : 07 Oct 2021 09:03
 Operator : SY/MD
 Sample : BFB211
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB211

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Oct 12 03:20:38 2021

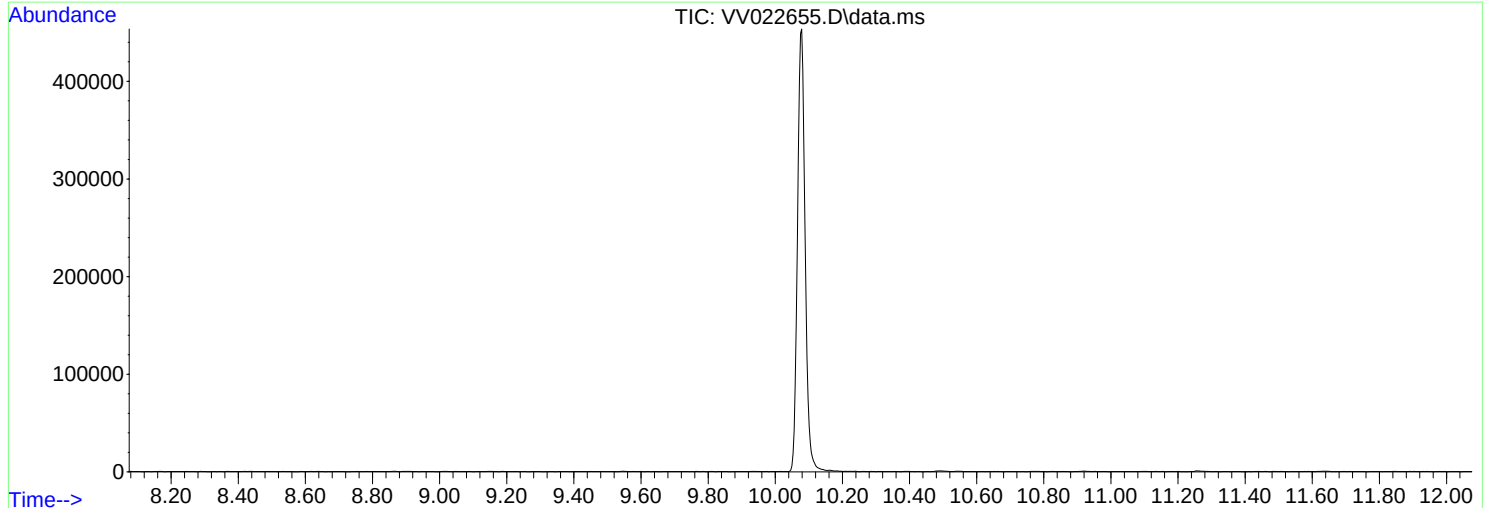

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	14478	PASS
75	95	30	80	49.3	42328	PASS
95	95	100	100	100.0	85816	PASS
96	95	5	9	6.6	5638	PASS
173	174	0.00	2	1.3	992	PASS
174	95	50	120	91.0	78056	PASS
175	174	5	9	7.7	6038	PASS
176	174	95	105	95.8	74749	PASS
177	176	5	10	6.6	4924	PASS

Scan 2797 (10.033 min): VV022655.D\data.ms
BFB211

m/z	Abundance
39.90	154.0
44.00	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	685.0
37.00	3077.0
38.00	3317.0
39.00	1338.0
39.90	146.0
44.00	455.0
45.00	666.0
46.10	154.0
47.00	807.0
48.00	530.0
49.00	2955.0
50.00	13822.0
51.00	4391.0
51.90	188.0
55.10	266.0
56.10	1043.0
57.00	2034.0
57.90	162.0
60.00	731.0
61.00	4065.0
62.00	3855.0
63.00	2809.0
64.10	417.0
65.00	676.0
66.00	140.0
67.00	221.0
68.00	7099.0
69.00	8263.0
70.00	718.0
71.90	457.0
73.00	3729.0
74.00	13385.0
75.00	39568.0
76.00	3465.0
76.90	452.0
77.80	284.0
78.90	2952.0
79.90	821.0
80.90	2788.0
82.00	751.0
83.00	101.0
85.80	125.0
87.00	3772.0
88.00	3178.0
90.90	344.0
92.00	2549.0
93.00	3790.0
94.00	9644.0
95.00	79768.0
96.00	5159.0
97.00	216.0
103.90	456.0
105.90	332.0
110.70	113.0
115.80	337.0
116.90	646.0
118.00	342.0
118.90	490.0
127.90	328.0
128.90	157.0
129.80	343.0
130.90	133.0
135.00	229.0
136.80	200.0
140.90	960.0
141.70	132.0
142.90	1126.0
144.80	236.0
145.80	146.0
147.90	245.0
153.00	125.0
154.90	188.0
157.00	140.0
160.70	147.0
170.80	124.0
172.00	1066.0
173.00	938.0
174.00	70904.0
175.00	5505.0
176.00	67184.0
177.00	4551.0
178.00	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	697.0
37.00	3347.0
38.00	3749.0
39.00	1461.0
39.90	162.0
44.00	521.0
45.00	715.0
46.10	172.0
47.00	859.0
47.90	574.0
49.00	3361.0
50.00	14936.0
51.00	4644.0
51.90	221.0
52.80	103.0
55.00	263.0
56.10	1086.0
57.00	2217.0
57.90	169.0
60.00	820.0
61.00	4400.0
62.00	4283.0
63.00	3115.0
64.00	435.0
65.00	639.0
66.00	167.0
67.00	240.0
68.00	7984.0
69.00	8910.0
70.00	818.0
71.90	473.0
73.00	4161.0
74.00	15153.0
75.00	43648.0
76.00	3685.0
76.90	504.0
77.90	335.0
78.90	3298.0
79.90	930.0
80.90	3218.0
82.00	803.0
83.00	140.0
85.80	128.0
87.00	4130.0
88.00	3682.0
90.90	376.0
92.00	2917.0
93.00	4209.0
94.00	10738.0
95.00	89008.0
96.00	5804.0
97.00	274.0
103.90	478.0
105.80	422.0
110.80	124.0
113.00	122.0
115.80	357.0
116.90	682.0
117.90	369.0
118.90	497.0
123.80	112.0
127.80	362.0
128.90	212.0
129.80	325.0
130.80	168.0
135.00	225.0
136.90	221.0
140.90	1110.0
141.80	160.0
142.90	1322.0
144.80	280.0
145.90	162.0
147.90	279.0
149.70	122.0
153.00	136.0
154.90	253.0
157.00	167.0
160.70	174.0
170.80	149.0
171.90	1039.0
173.00	1028.0
174.00	80712.0
175.00	6230.0
176.00	77104.0
177.00	5072.0
178.00	267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	713.0
37.00	3349.0
38.00	3795.0
39.00	1450.0
39.90	178.0
44.00	582.0
45.00	719.0
46.20	173.0
47.00	869.0
47.90	546.0
49.10	3289.0
50.00	14675.0
51.00	4479.0
51.90	204.0
52.90	105.0
55.00	228.0
56.10	1026.0
57.00	2205.0
57.90	148.0
60.00	780.0
61.00	4374.0
62.00	4171.0
63.00	3216.0
64.00	494.0
64.90	639.0
66.00	156.0
67.00	229.0
68.00	8197.0
69.00	8472.0
70.00	821.0
72.00	471.0
73.00	3971.0
74.00	15313.0
75.00	43768.0
76.00	3519.0
76.90	460.0
77.90	373.0
78.90	3292.0
79.90	952.0
80.90	3405.0
81.90	774.0
83.00	160.0
85.80	113.0
87.00	4098.0
88.00	3817.0
90.90	373.0
92.00	2961.0
93.00	4265.0
94.00	10664.0
95.00	88672.0
96.00	5950.0
97.00	260.0
103.90	448.0
105.90	457.0
110.80	118.0
112.10	111.0
113.00	127.0
114.80	108.0
115.80	376.0
116.90	683.0
117.90	379.0
118.90	496.0
123.80	113.0
127.80	383.0
128.90	212.0
129.80	253.0
130.80	160.0
135.00	208.0
136.90	241.0
140.90	1152.0
141.80	179.0
142.90	1401.0
143.80	102.0
144.80	287.0
145.80	174.0
147.90	278.0
149.80	130.0
152.90	107.0
154.90	266.0
157.00	163.0
160.80	156.0
170.80	144.0
171.90	994.0
173.00	1011.0
174.00	82552.0
175.00	6378.0
176.00	79960.0
177.00	5150.0
177.90	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211