

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100818\
 Data File : VV008170.D
 Acq On : 08 Oct 2018 23:24
 Operator : SY/MD
 Sample : J5280-04
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ1

Quant Time: Oct 09 09:30:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 04:07:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	82348	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	79392	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	36197	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	25614	5.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.40%
7) Chloroethane-d5	1.59	69	21186	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.40%
11) 1,1-Dichloroethene-d2	2.14	63	37732	3.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.20%
20) 2-Butanone-d5	3.96	46	64842	53.32	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.64%
24) Chloroform-d	4.41	84	52827	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.09	65	26454	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
32) Benzene-d6	5.10	84	102231	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	32670	5.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.60%
41) Toluene-d8	7.36	98	89266	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.67	79	10803	4.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.40%
46) 2-Hexanone-d5	8.14	63	39338	44.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.12%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22133	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	36252	5.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	2341	2.841 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008170.D
Acq On : 08 Oct 2018 23:24
Operator : SY/MD
Sample : J5280-04
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYJ1

Quant Time: Oct 09 09:30:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 09 04:07:48 2018
Response via : Initial Calibration

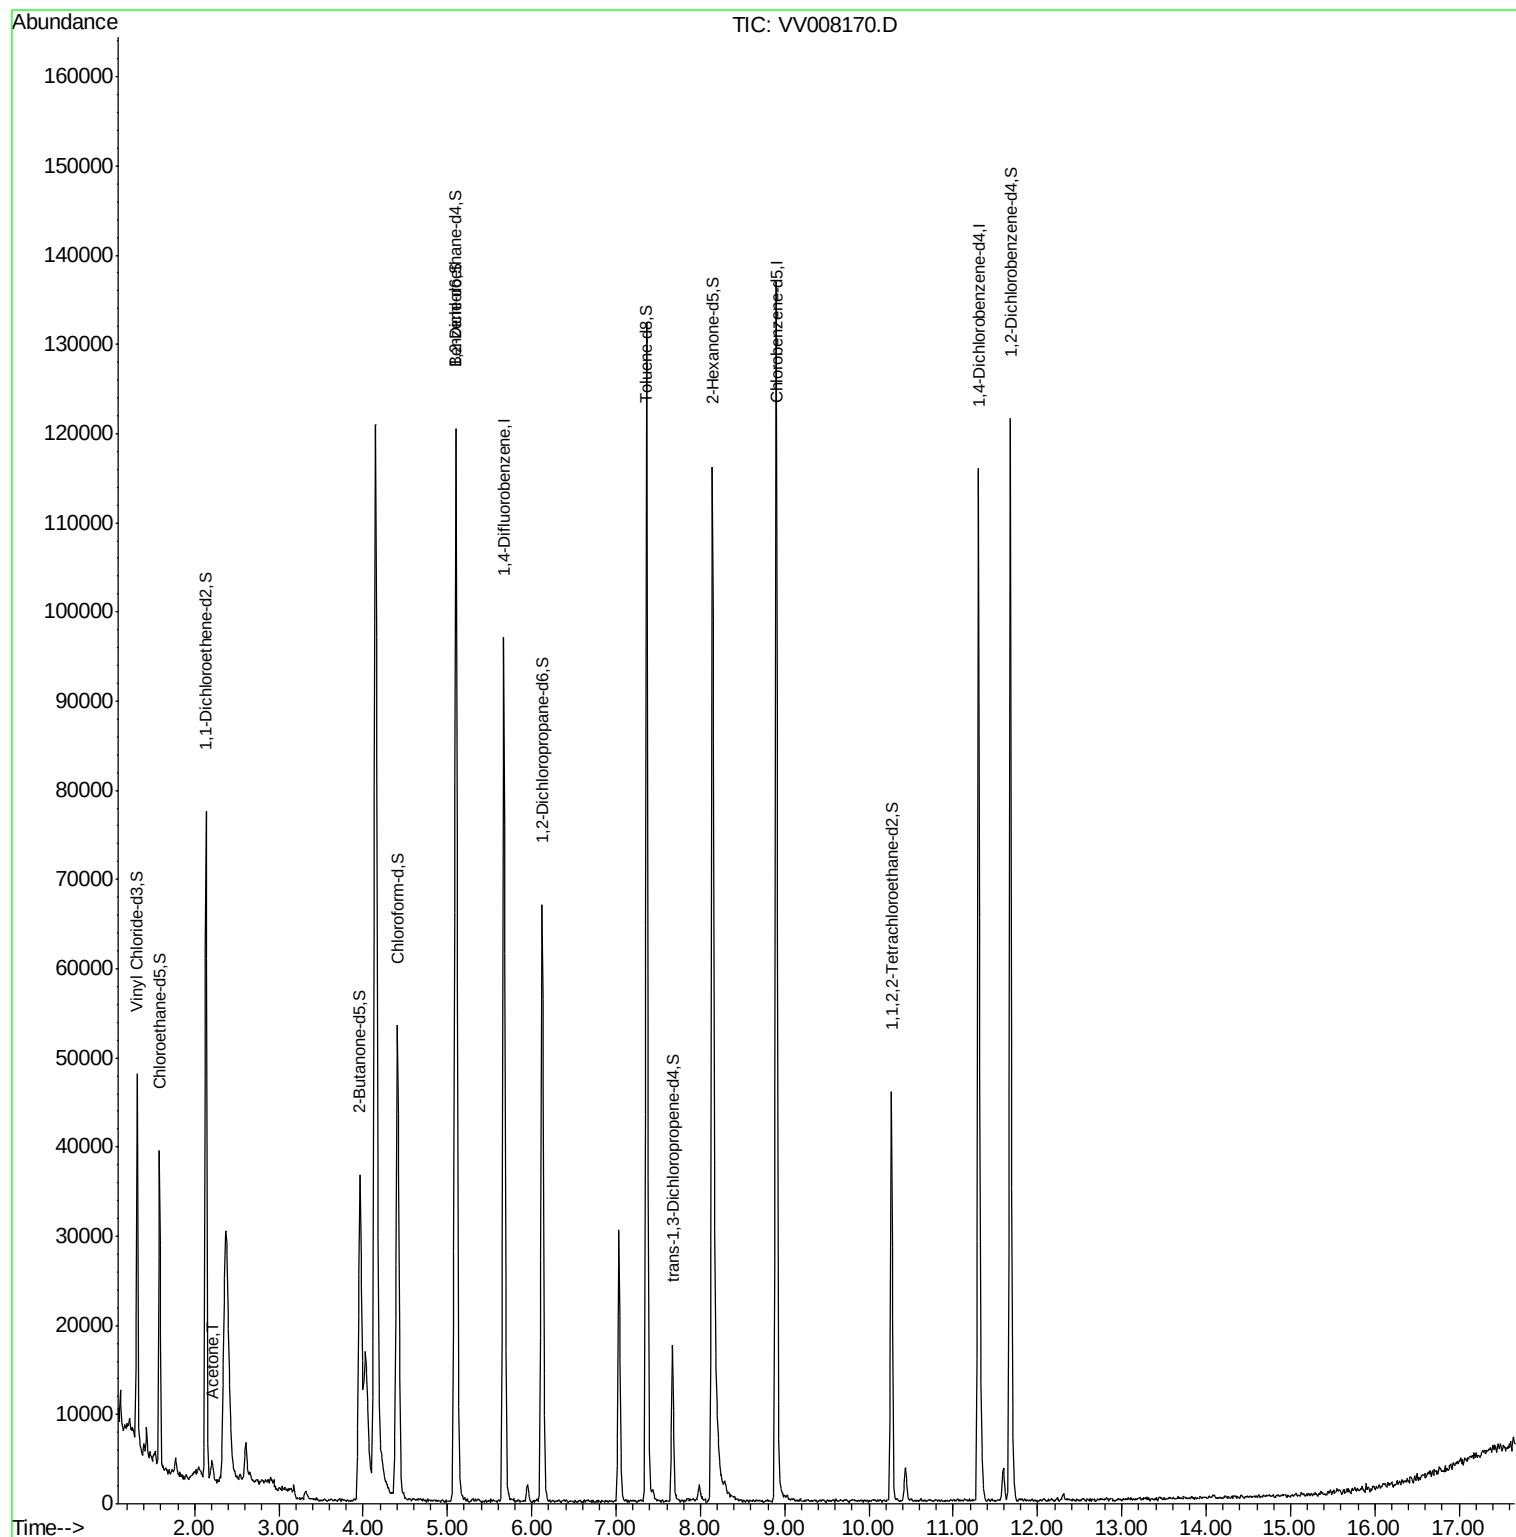

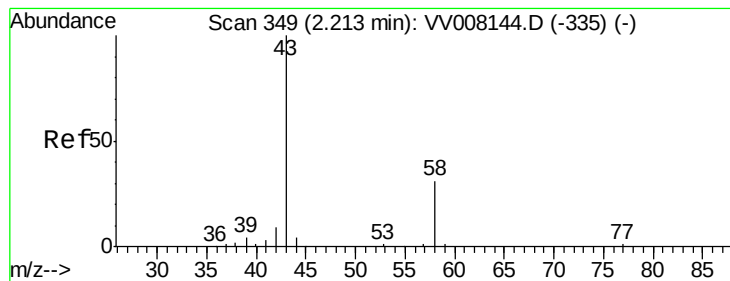

#13

Acetone

Concen: 2.841 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.00 min

Lab File: VV008170.D

Acq: 08 Oct 2018 23:24

Instrument :
MSVOA_V
ClientSampleId :
BEYJ1

Tot Ion: 43 Resp: 2341

Ion Ratio Lower Upper

43 100

58 31.6 0.0 62.2

