

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100818\
 Data File : VV008171.D
 Acq On : 08 Oct 2018 23:51
 Operator : SY/MD
 Sample : J5280-05
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ2

Quant Time: Oct 09 09:31:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 04:07:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	87777	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	83082	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	36959	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24910	4.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.40%
7) Chloroethane-d5	1.59	69	21227	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.14	63	37367	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	3.96	46	65485	50.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.04%
24) Chloroform-d	4.41	84	52011	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.09	65	26367	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.10	84	101783	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.13	67	32155	4.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.60%
41) Toluene-d8	7.36	98	87922	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
43) trans-1,3-Dichloropropene-	7.67	79	9960	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.14	63	38512	41.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.44%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21475	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	35480	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	3043	3.465 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008171.D
Acq On : 08 Oct 2018 23:51
Operator : SY/MD
Sample : J5280-05
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYJ2

Quant Time: Oct 09 09:31:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 09 04:07:48 2018
Response via : Initial Calibration

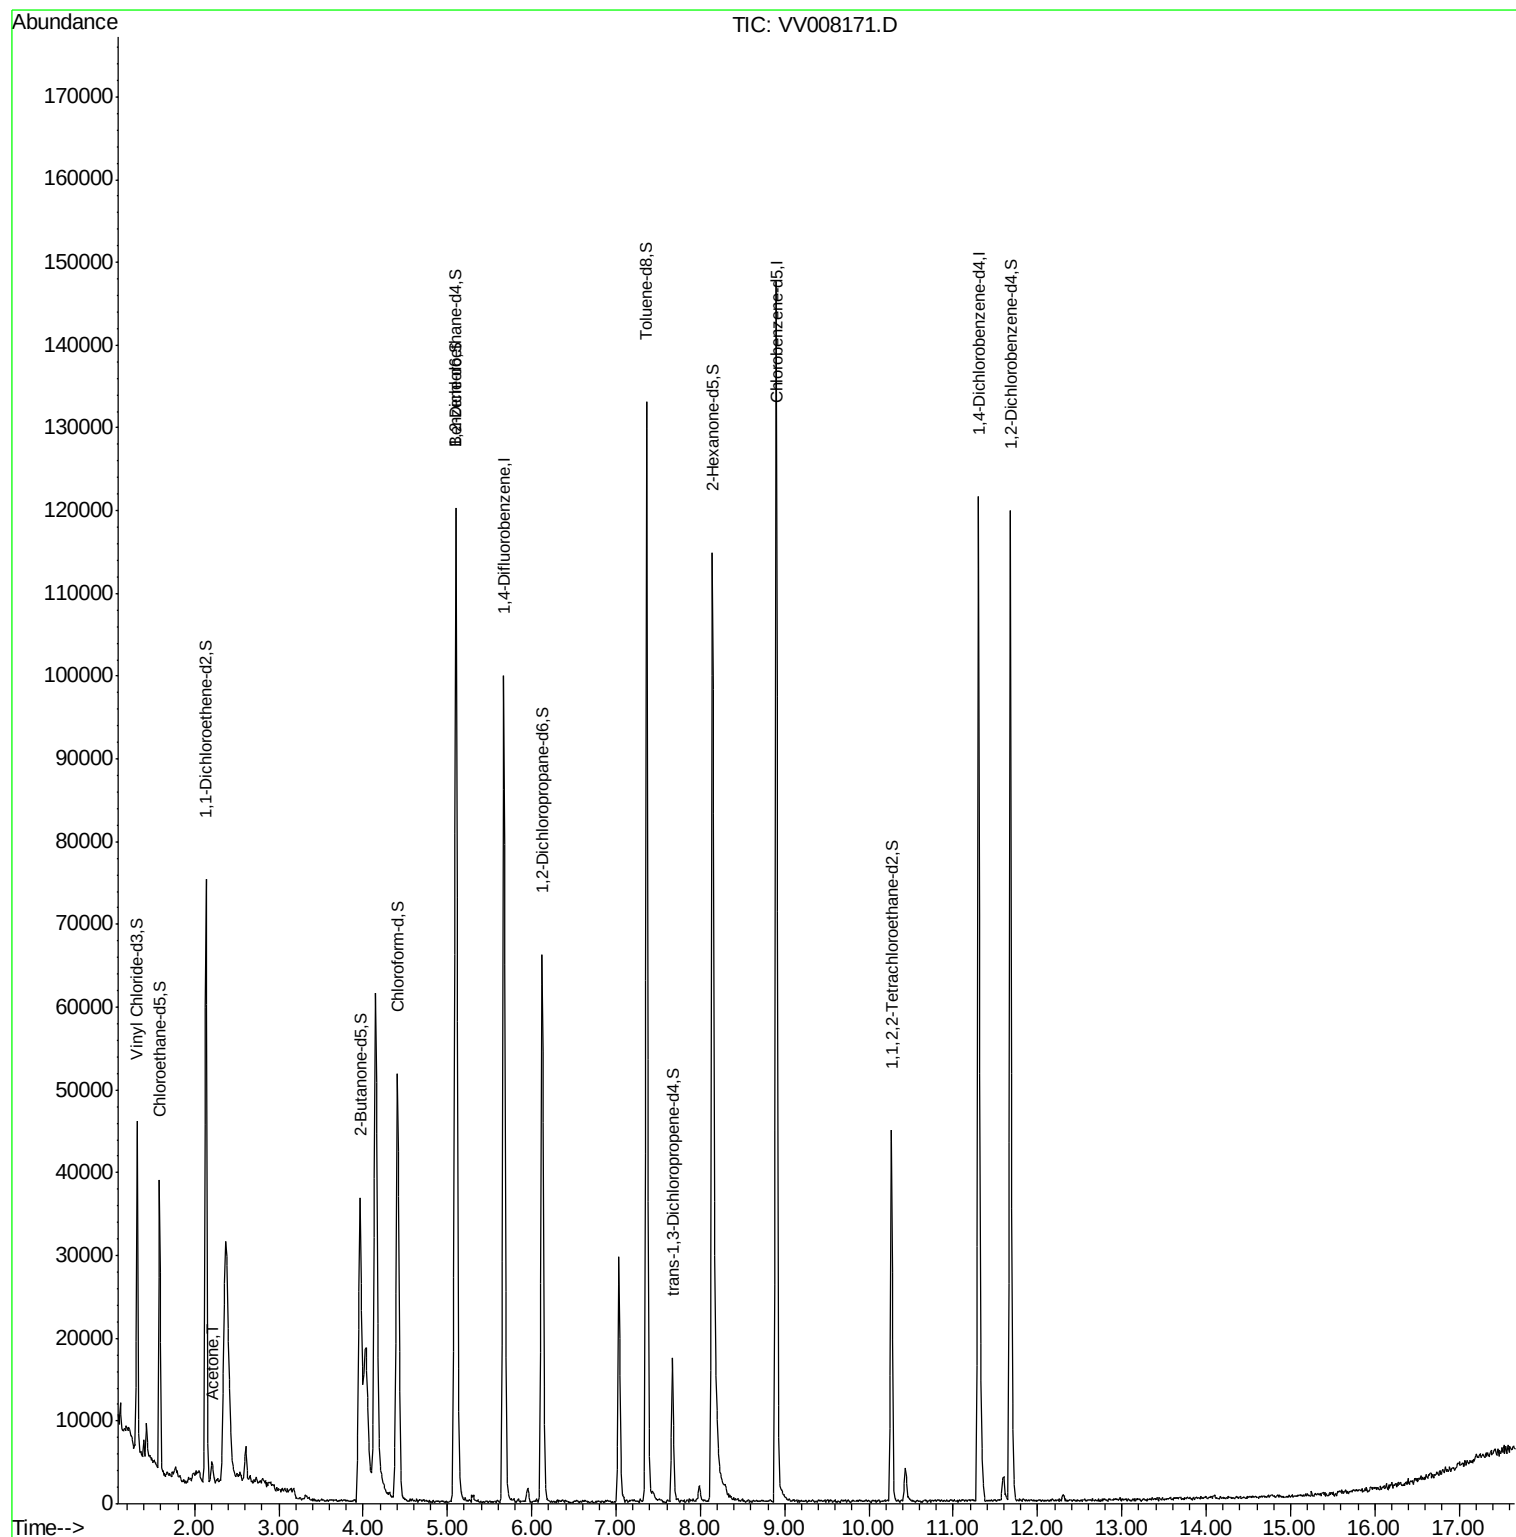

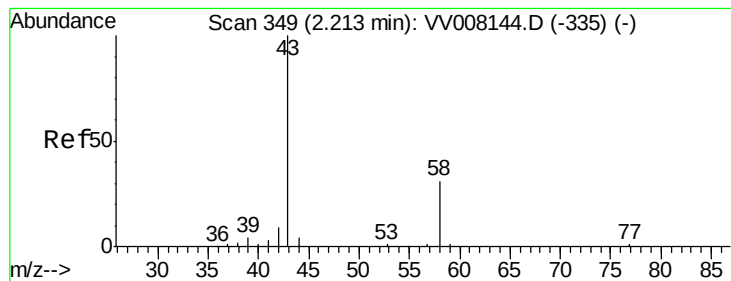

#13
 Acetone
 Concen: 3.465 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. 0.00 min
 Lab File: VV008171.D
 Acq: 08 Oct 2018 23:51

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ2

Tot Ion: 43 Resp: 3043
 Ion Ratio Lower Upper
 43 100
 58 28.5 0.0 62.2

