

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100818\
 Data File : VV008175.D
 Acq On : 09 Oct 2018 01:41
 Operator : SY/MD
 Sample : J5280-09
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ6

Quant Time: Oct 09 09:35:32 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 04:07:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	84381	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	81339	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	35358	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	26188	5.06	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.20%
7) Chloroethane-d5	1.59	69	21986	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.14	63	38282	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	3.96	46	65026	52.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.36%
24) Chloroform-d	4.41	84	54165	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.09	65	28163	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.10	84	104781	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	33092	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.36	98	92390	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.67	79	10265	4.47	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.40%
46) 2-Hexanone-d5	8.14	63	40697	44.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21837	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	35642	5.31	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	2577	3.052 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008175.D
Acq On : 09 Oct 2018 01:41
Operator : SY/MD
Sample : J5280-09
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYJ6

Quant Time: Oct 09 09:35:32 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 09 04:07:48 2018
Response via : Initial Calibration

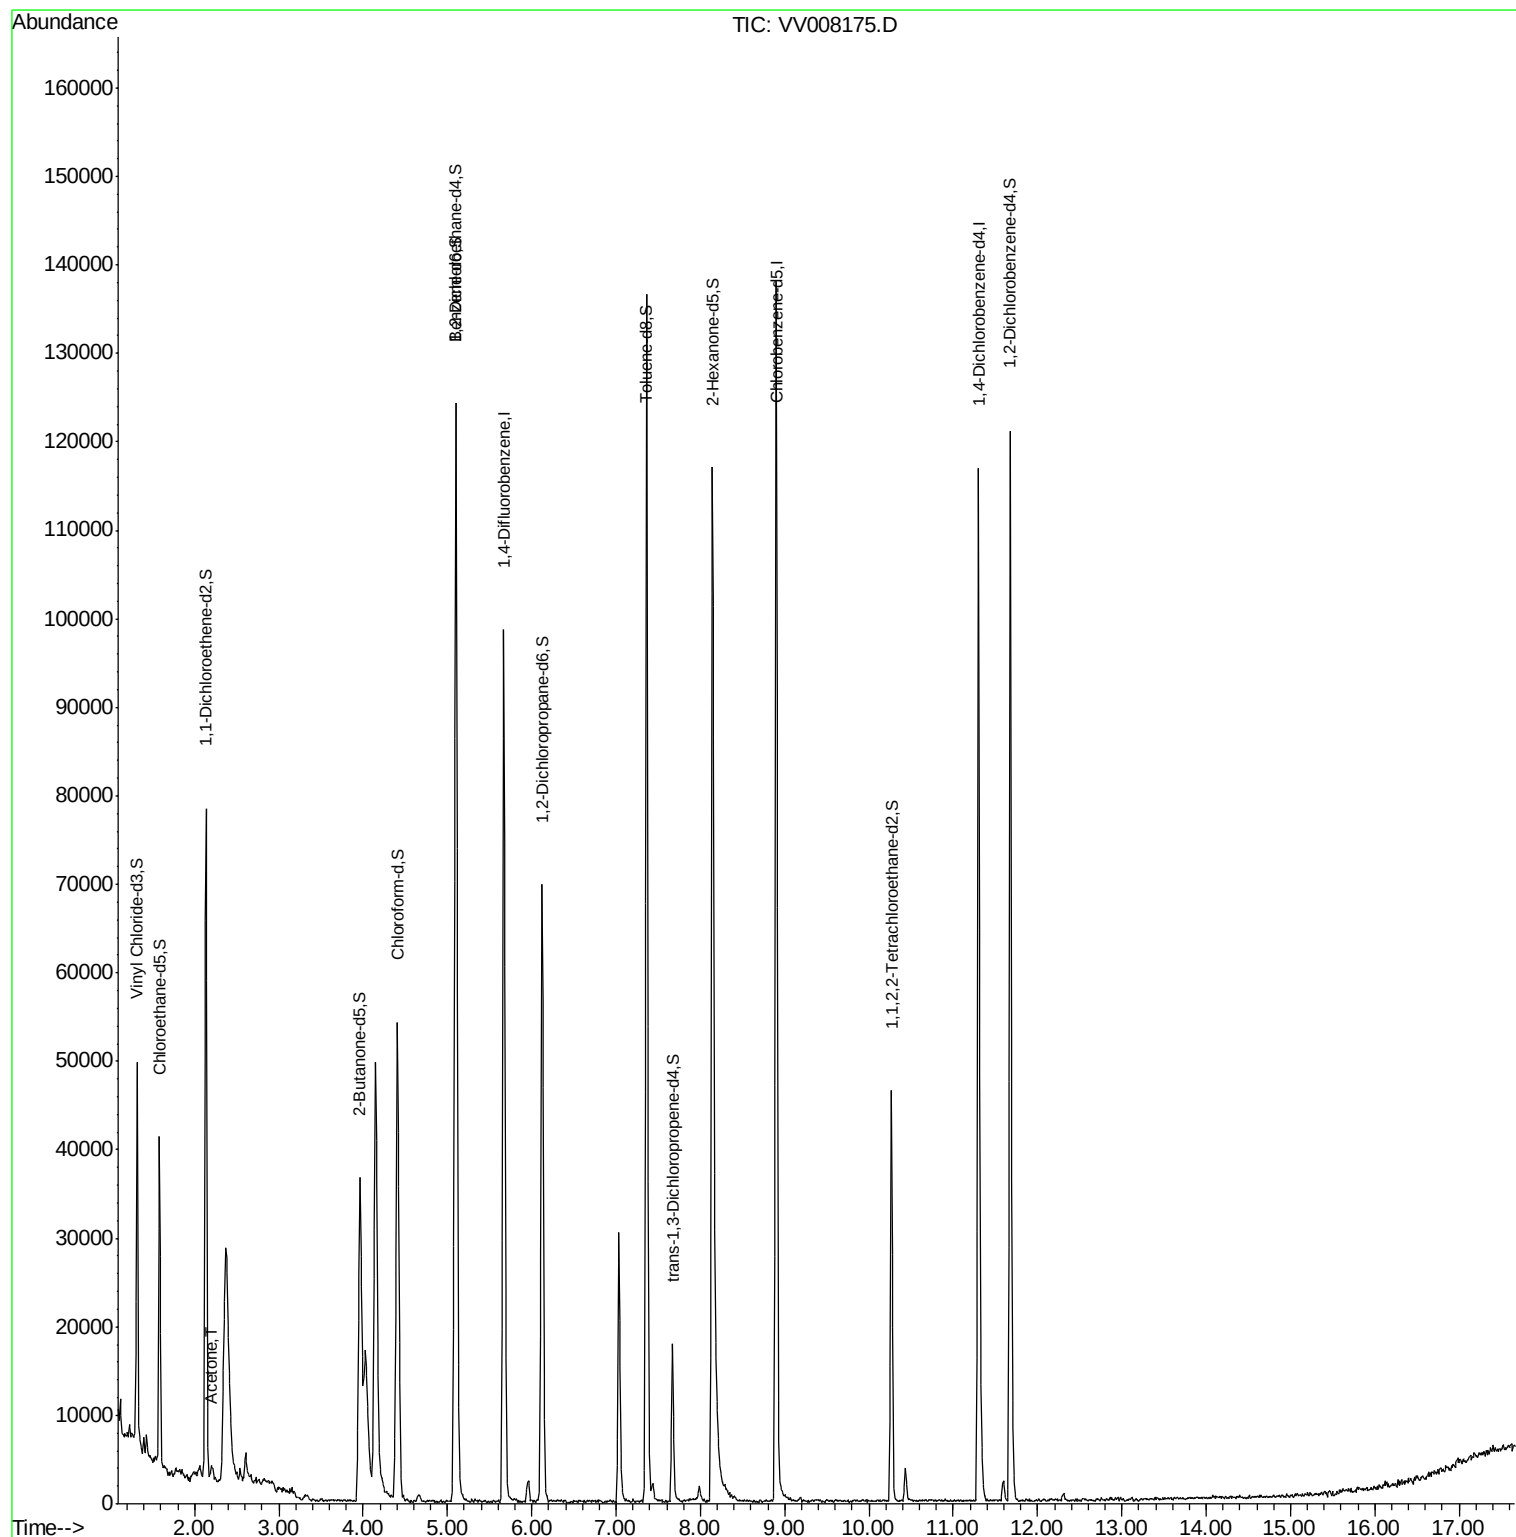

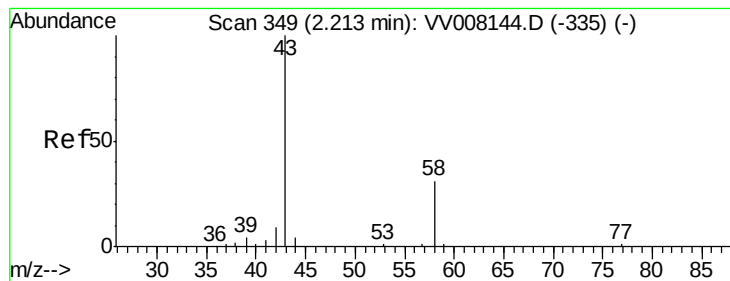

#13
 Acetone
 Concen: 3.052 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. -0.00 min
 Lab File: VV008175.D
 Acq: 09 Oct 2018 01:41

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ6

Tot Ion: 43 Resp: 2577
 Ion Ratio Lower Upper
 43 100
 58 23.7 0.0 62.2

