

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100818\
 Data File : VV008178.D
 Acq On : 09 Oct 2018 03:03
 Operator : SY/MD
 Sample : J5280-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ9

Quant Time: Oct 09 09:37:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 04:07:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	81917	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	79760	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	35802	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24578	4.89	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.80%
7) Chloroethane-d5	1.59	69	21343	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.14	63	36851	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.96	46	62216	51.43	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.86%
24) Chloroform-d	4.41	84	51431	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.09	65	26379	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.10	84	99535	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.13	67	31890	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.36	98	87893	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	7.67	79	9777	4.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.80%
46) 2-Hexanone-d5	8.14	63	38860	43.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.66%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	21729	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	35099	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	2201	2.685 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008178.D
Acq On : 09 Oct 2018 03:03
Operator : SY/MD
Sample : J5280-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYJ9

Quant Time: Oct 09 09:37:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 09 04:07:48 2018
Response via : Initial Calibration

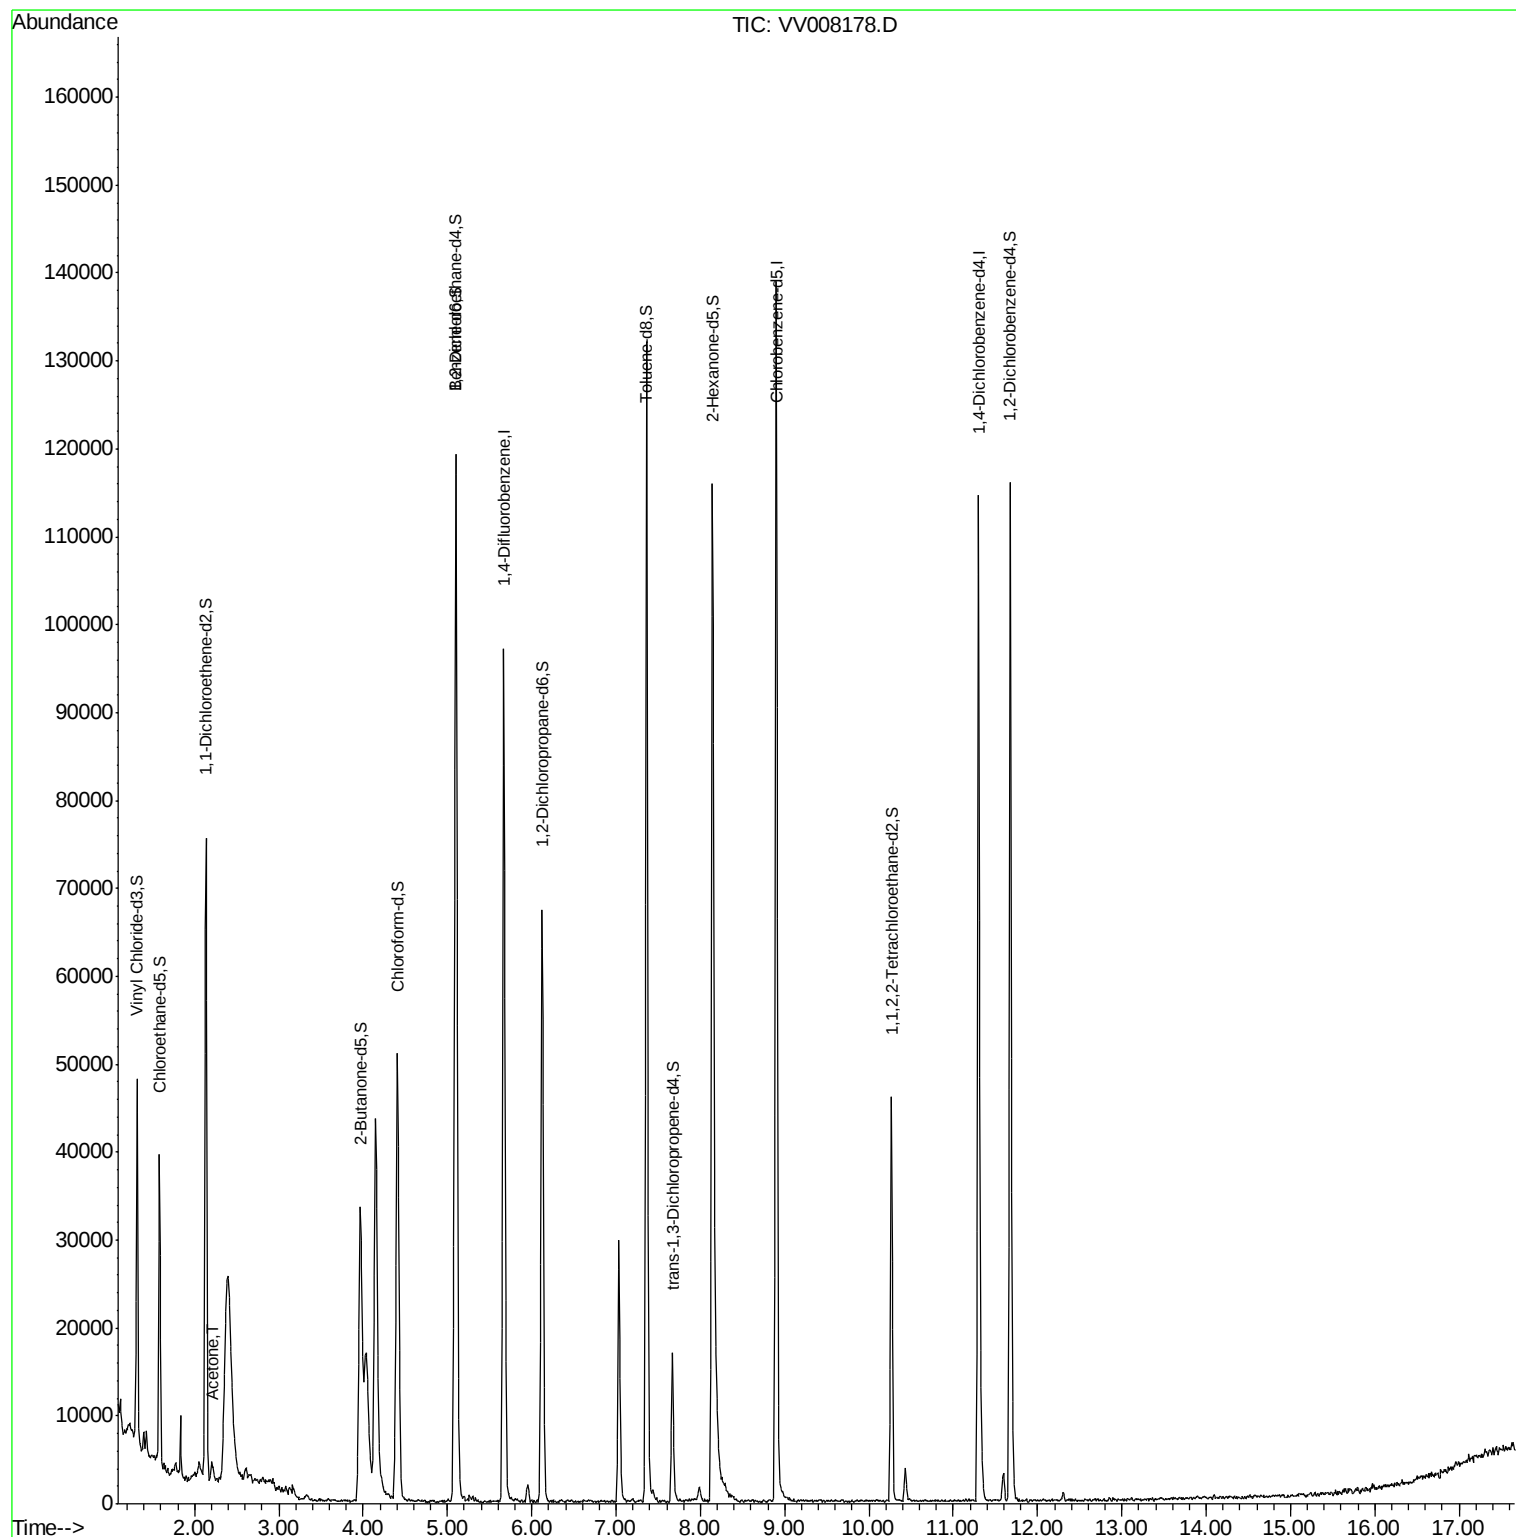

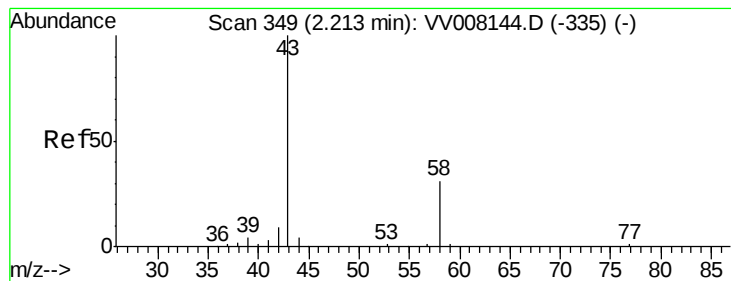

#13
 Acetone
 Concen: 2.685 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. 0.00 min
 Lab File: VV008178.D
 Acq: 09 Oct 2018 03:03

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYJ9

Tot Ion: 43 Resp: 2201
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 62.2

