

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100818\
 Data File : VV008183.D
 Acq On : 09 Oct 2018 05:19
 Operator : SY/MD
 Sample : J5280-17
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYK4

Quant Time: Oct 09 09:30:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 09 04:07:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	83643	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	80491	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	36295	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24594	4.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.80%
7) Chloroethane-d5	1.59	69	20694	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.60%
11) 1,1-Dichloroethene-d2	2.14	63	36438	3.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.60%
20) 2-Butanone-d5	3.97	46	62515	50.61	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.22%
24) Chloroform-d	4.41	84	51785	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.09	65	26128	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.10	84	98383	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.12	67	31538	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	85914	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
43) trans-1,3-Dichloropropene-	7.67	79	9584	4.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.40%
46) 2-Hexanone-d5	8.14	63	38264	42.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.56%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	20989	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	34912	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%


Target Compounds					Ovalue
13) Acetone	2.22	43	2598	3.104 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008183.D
Acq On : 09 Oct 2018 05:19
Operator : SY/MD
Sample : J5280-17
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYK4

Quant Time: Oct 09 09:30:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 09 04:07:48 2018
Response via : Initial Calibration

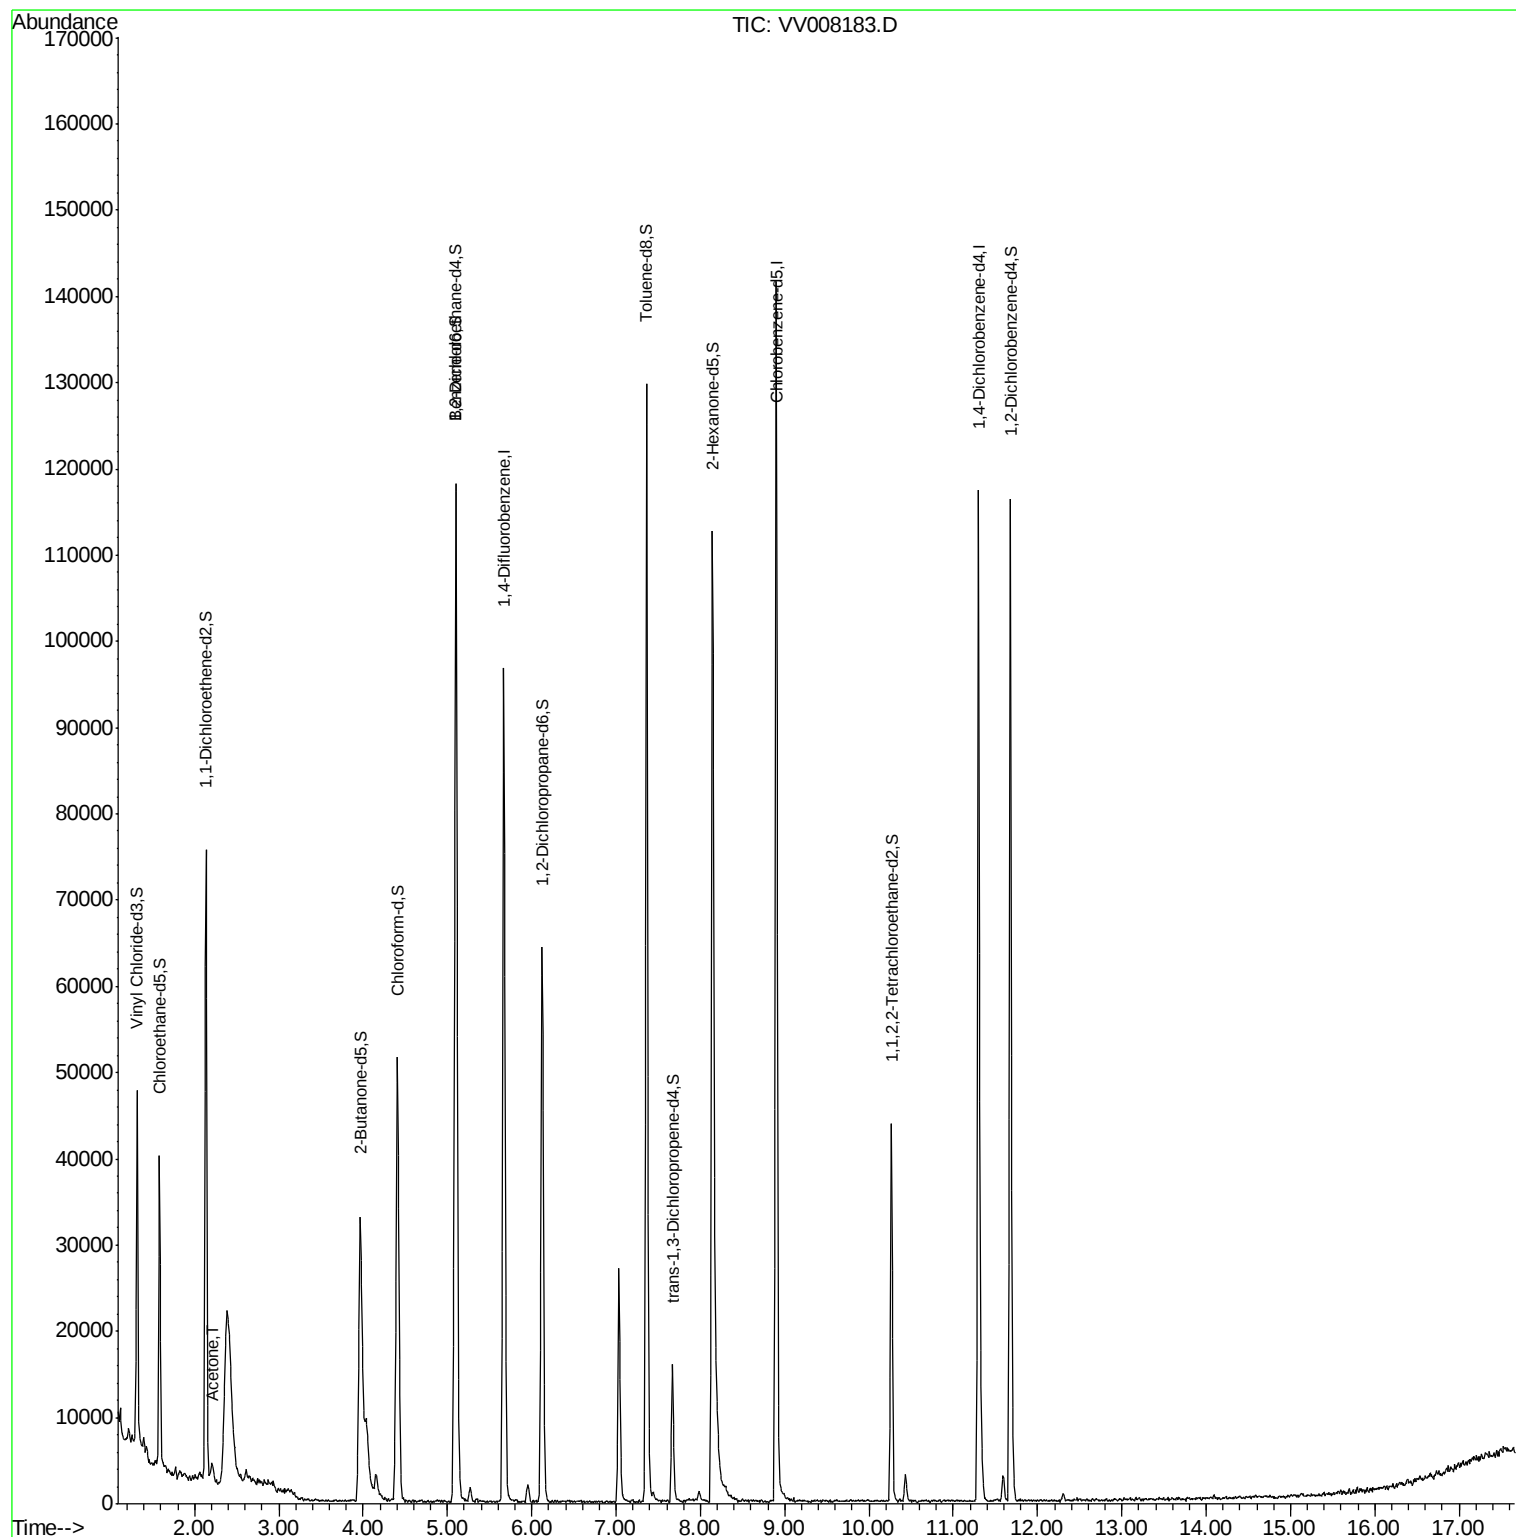

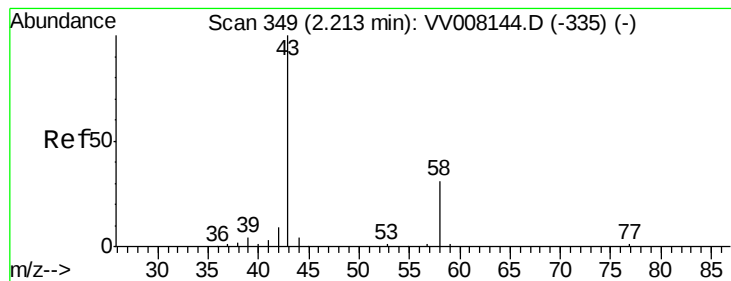

#13
 Acetone
 Concen: 3.104 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. 0.00 min
 Lab File: VV008183.D
 Acq: 09 Oct 2018 05:19

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYK4

Tot Ion: 43 Resp: 2598
 Ion Ratio Lower Upper
 43 100
 58 26.2 0.0 62.2

