

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100818\
 Data File : VV008147.D
 Acq On : 08 Oct 2018 12:27
 Operator : SY/MD
 Sample : J5277-20
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYD7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	84	rVB	43453	49690	17.80%	2.070%
2	1.586	146	154	167	rVB	35339	40255	14.42%	1.677%
3	2.135	315	325	336	rVB	74899	105911	37.94%	4.413%
4	2.380	383	401	430	rBV	9868	43902	15.72%	1.829%
5	3.968	879	895	910	rBV2	34374	98501	35.28%	4.104%
6	4.155	945	953	971	rVB3	2283	5349	1.92%	0.223%
7	4.405	1014	1031	1052	rBV	51154	122390	43.84%	5.100%
8	5.100	1230	1247	1274	rBV2	121196	279189	100.00%	11.633%
9	5.669	1410	1424	1440	rBV	97994	189737	67.96%	7.906%
10	6.122	1552	1565	1587	rBV	66995	135025	48.36%	5.626%
11	7.036	1837	1849	1864	rBV2	32177	56347	20.18%	2.348%
12	7.363	1935	1951	1970	rBV	136266	234672	84.05%	9.778%
13	7.669	2035	2046	2068	rVB	19522	32894	11.78%	1.371%
14	7.984	2134	2144	2157	rVB2	4139	7693	2.76%	0.321%
15	8.145	2181	2194	2222	rBV2	116995	252357	90.39%	10.515%
16	8.900	2417	2429	2446	rBV	137257	228696	81.91%	9.529%
17	10.267	2843	2854	2866	rBV2	45802	72089	25.82%	3.004%
18	10.431	2896	2905	2926	rVB	13237	25100	8.99%	1.046%
19	11.299	3164	3175	3200	rBV	124991	211865	75.89%	8.828%
20	11.592	3259	3266	3274	rBV5	1687	2865	1.03%	0.119%
21	11.675	3281	3292	3314	rVB	121897	205431	73.58%	8.560%


Sum of corrected areas: 2399958

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008147.D
Acq On : 08 Oct 2018 12:27
Operator : SY/MD
Sample : J5277-20
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

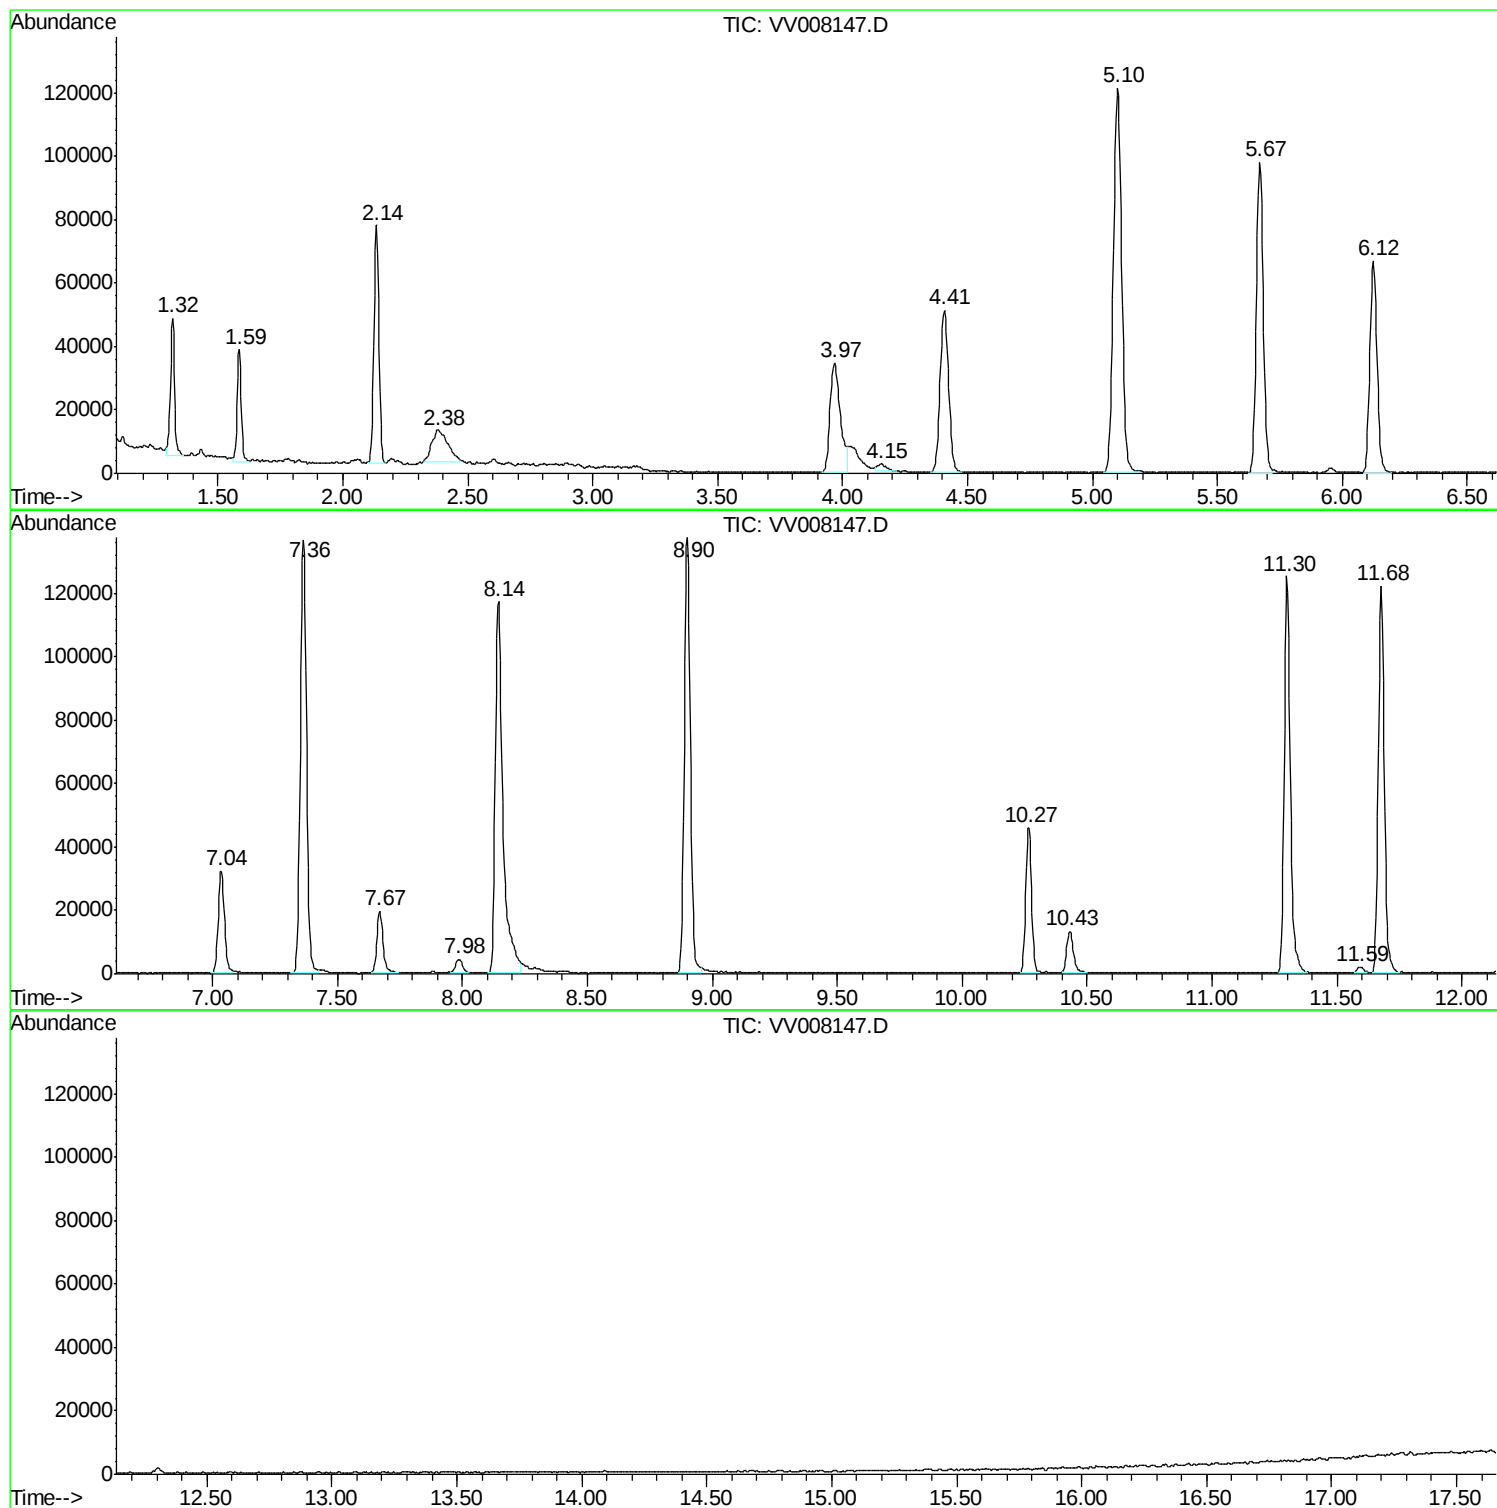

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100818\
Data File : VV008147.D
Acq On : 08 Oct 2018 12:27
Operator : SY/MD
Sample : J5277-20
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYD7










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.38	1.16 ug/L	43902	1,4-Difluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	43
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	43
3			Formamide	45	CH3NO	000075-12-7	5
4			Ethylamine	45	C2H7N	000075-04-7	5
5			Formamide	45	CH3NO	000075-12-7	4

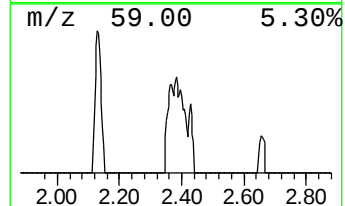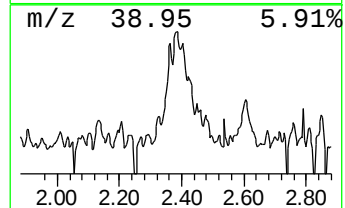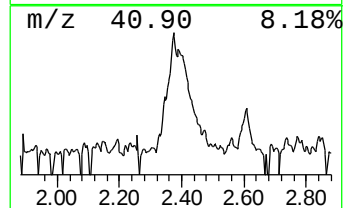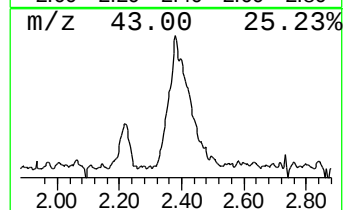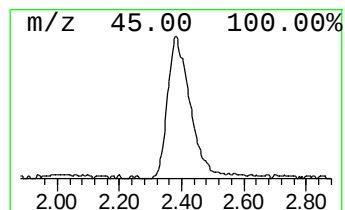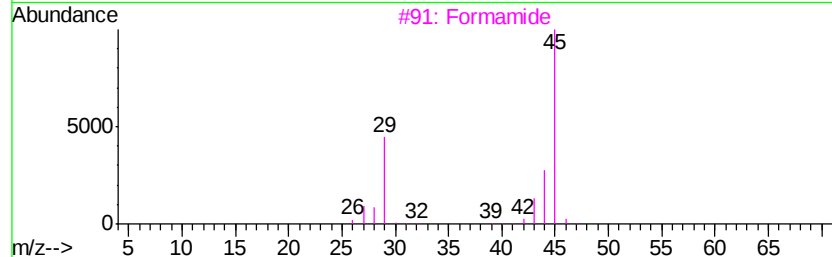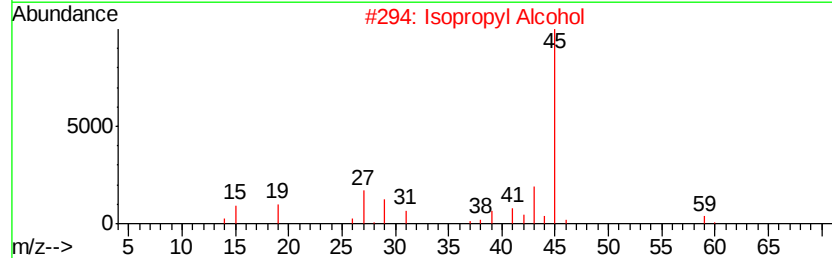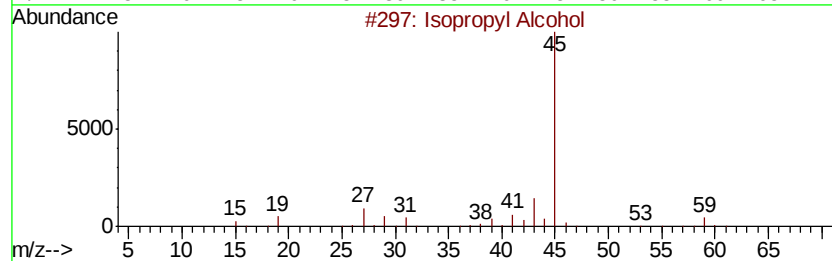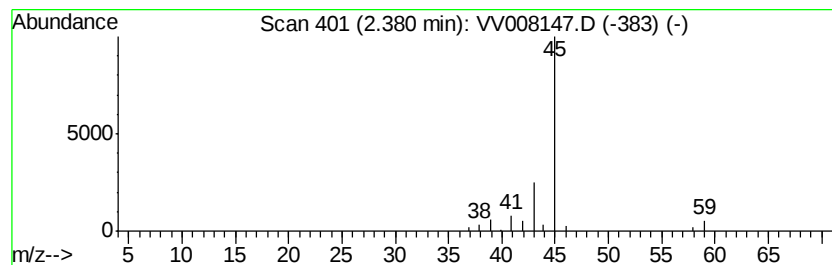

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100818\
Data File : VV008147.D
Acq On : 08 Oct 2018 12:27
Operator : SY/MD
Sample : J5277-20
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYD7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	2.38	1.2	ug/L	43902	1	5.67	189737	5.0