


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100818\
Data File : VV008143.D
Acq On : 08 Oct 2018 09:50
Operator : SY/MD
Sample : BFB83
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB83

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 09 04:07:48 2018

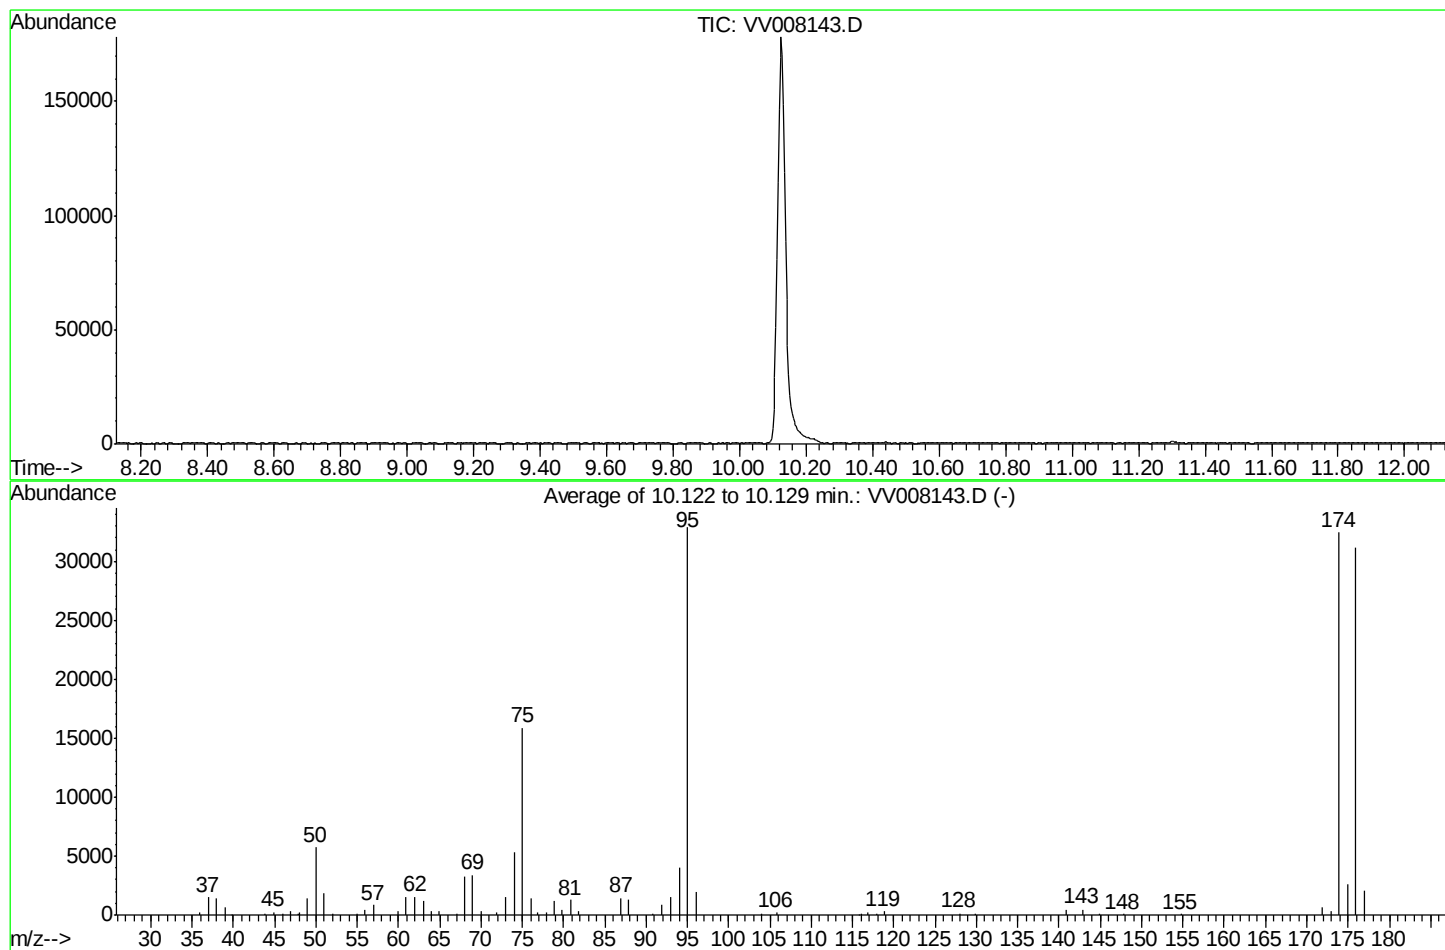

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	5735	PASS
75	95	30	80	48.3	15886	PASS
95	95	100	100	100.0	32885	PASS
96	95	5	9	6.1	2007	PASS
173	174	0.00	2	1.1	371	PASS
174	95	50	120	98.8	32506	PASS
175	174	5	9	8.1	2647	PASS
176	174	95	101	95.9	31186	PASS
177	176	5	9	6.8	2108	PASS

Scan 2796 (10.080 min): VV008143.D
BFB83

m/z	Abundance
39.80	108.0
43.90	267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.90	250.0
36.90	1521.0
38.00	1382.0
38.90	637.0
39.90	133.0
43.90	404.0
44.80	244.0
46.00	107.0
47.00	369.0
47.80	221.0
48.00	225.0
48.90	1383.0
50.00	5787.0
51.00	1875.0
52.00	118.0
55.00	133.0
55.90	450.0
57.00	875.0
60.00	342.0
61.00	1433.0
62.00	1517.0
63.00	1219.0
64.00	305.0
65.00	383.0
68.00	3329.0
69.00	3170.0
69.90	322.0
71.90	253.0
72.90	1510.0
74.00	5451.0
75.00	15806.0
76.00	1488.0
76.90	228.0
78.00	201.0
78.90	1160.0
79.80	408.0
80.90	1228.0
81.90	307.0
87.00	1366.0
87.90	1257.0
90.80	168.0
91.90	891.0
93.00	1557.0
94.00	4171.0
95.00	32320.0
96.00	2028.0
103.90	167.0
105.80	178.0
116.00	104.0
116.80	244.0
117.90	138.0
118.80	252.0
127.90	156.0
129.90	110.0
140.90	359.0
142.80	518.0
144.90	150.0
171.90	639.0
172.90	522.0
173.90	31512.0
174.90	2599.0
175.90	29864.0
176.90	2008.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.90	270.0
37.00	1523.0
38.00	1468.0
38.90	645.0
39.90	135.0
43.90	396.0
44.80	262.0
45.90	117.0
47.00	363.0
47.90	240.0
48.90	1410.0
50.00	5910.0
51.00	1969.0
52.00	114.0
54.90	138.0
55.90	489.0
57.00	870.0
60.00	365.0
60.90	1600.0
62.00	1634.0
63.00	1271.0
64.00	300.0
65.00	331.0
67.10	120.0
68.00	3326.0
69.00	3487.0
70.00	351.0
71.90	249.0
72.90	1587.0
74.00	5425.0
75.00	16432.0
76.00	1503.0
76.90	182.0
77.80	191.0
78.90	1212.0
79.80	411.0
80.90	1318.0
81.80	346.0
87.00	1507.0
87.90	1326.0
90.80	180.0
91.90	914.0
92.90	1564.0
94.00	4150.0
95.00	33984.0
96.00	2071.0
103.90	148.0
105.80	176.0
116.10	106.0
116.90	272.0
117.90	132.0
118.80	291.0
128.00	173.0
129.90	115.0
140.80	405.0
142.80	476.0
144.90	126.0
147.80	108.0
154.80	124.0
171.90	716.0
173.00	591.0
173.90	33568.0
174.90	2736.0
175.90	32128.0
176.90	2165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.90	264.0
37.00	1406.0
37.90	1407.0
39.00	605.0
39.90	126.0
43.90	413.0
44.90	274.0
45.90	115.0
47.00	344.0
47.90	237.0
49.00	1311.0
50.00	5508.0
51.00	1858.0
52.00	106.0
54.90	118.0
55.90	507.0
57.00	781.0
59.90	367.0
61.00	1557.0
62.00	1564.0
63.00	1225.0
64.00	251.0
64.90	326.0
67.10	117.0
68.00	3081.0
69.00	3467.0
69.90	342.0
71.90	232.0
72.90	1480.0
74.00	5075.0
75.00	15420.0
76.00	1337.0
76.80	148.0
77.80	164.0
78.90	1109.0
79.80	393.0
80.80	1277.0
81.80	318.0
86.90	1452.0
87.90	1296.0
90.80	149.0
91.90	890.0
92.90	1444.0
94.00	3811.0
95.00	32352.0
96.00	1923.0
103.90	140.0
105.80	153.0
115.70	126.0
116.00	112.0
116.80	257.0
117.90	108.0
118.90	301.0
128.00	161.0
129.90	119.0
140.80	447.0
142.80	460.0
145.00	120.0
147.80	105.0
154.70	130.0
171.90	705.0
173.90	32440.0
174.90	2607.0
175.90	31568.0
176.90	2151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83