


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100820\
 Data File : VV018756.D
 Acq On : 08 Oct 2020 09:37
 Operator : SY/MD
 Sample : BFB60
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 09 07:09:39 2020

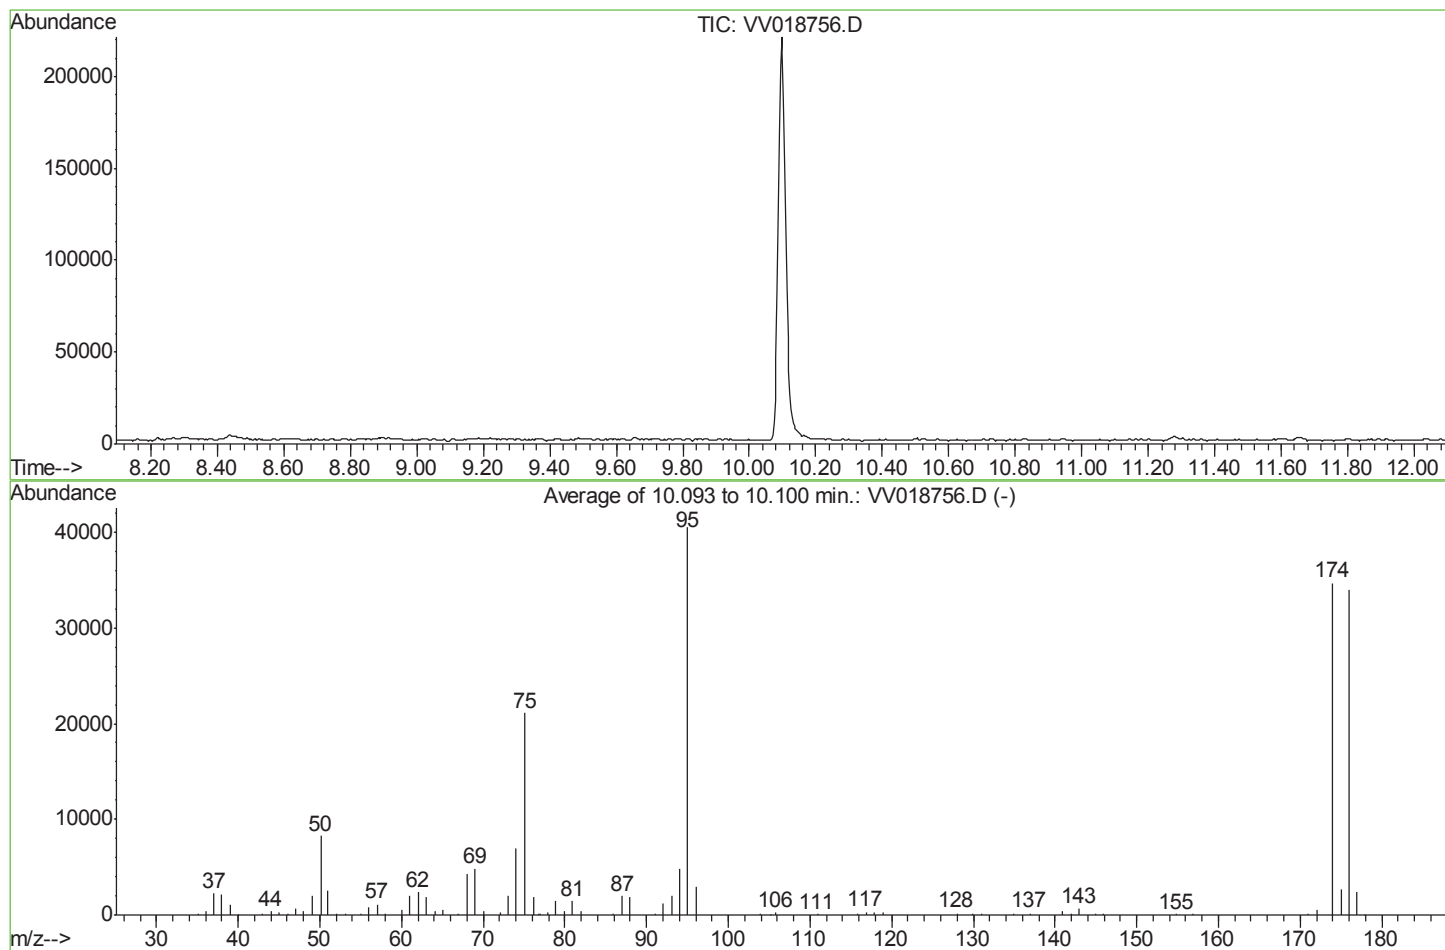

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	8268	PASS
75	95	30	80	52.0	21080	PASS
95	95	100	100	100.0	40520	PASS
96	95	5	9	7.3	2963	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	34666	PASS
175	174	5	9	7.8	2704	PASS
176	174	95	101	98.0	33973	PASS
177	176	5	9	7.1	2414	PASS

m/z	Abundance
35.10	137.0
36.00	360.0
37.00	2106.0
38.00	2167.0
39.00	869.0
40.00	446.0
43.00	153.0
44.00	1677.0
44.90	305.0
46.10	164.0
47.10	556.0
48.00	330.0
49.00	1962.0
50.10	8488.0
51.00	2533.0
52.20	125.0
53.10	105.0
55.00	176.0
56.00	820.0
57.10	1017.0
58.10	118.0
60.00	472.0
61.00	2007.0
62.00	2295.0
63.00	1747.0
64.10	332.0
65.00	508.0
66.90	183.0
68.00	4251.0
69.00	4640.0
70.00	363.0
72.10	314.0
73.00	2149.0
74.00	7068.0
75.10	20736.0
76.10	1892.0
76.80	297.0
77.80	298.0
78.90	1441.0
80.00	481.0
80.90	1432.0
82.00	382.0
87.00	1983.0
88.00	1756.0
91.00	166.0
92.00	1363.0
93.10	1710.0
94.00	4738.0
95.10	39104.0
96.00	2830.0
103.90	200.0
105.90	226.0
115.80	156.0
116.90	379.0
117.80	217.0
118.90	292.0
128.00	193.0
129.90	200.0
131.00	103.0
135.00	112.0
136.90	142.0
140.80	493.0
142.00	138.0
143.00	736.0
145.00	172.0
156.90	120.0
171.10	137.0
172.00	485.0
174.00	32776.0
175.00	2512.0
176.00	31992.0
177.00	2273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.10	123.0
36.00	498.0
37.10	2270.0
38.00	2296.0
39.00	1045.0
39.90	452.0
43.00	140.0
44.00	1636.0
44.90	313.0
46.10	192.0
47.10	740.0
47.90	382.0
49.00	2026.0
50.10	8574.0
51.00	2774.0
52.10	117.0
53.10	129.0
55.10	174.0
56.00	897.0
57.00	1149.0
58.00	180.0
60.00	507.0
61.00	1988.0
62.00	2469.0
63.00	1882.0
64.10	355.0
65.00	610.0
66.90	209.0
68.00	4438.0
69.00	4989.0
70.00	411.0
72.10	370.0
73.00	2126.0
74.00	7276.0
75.10	21648.0
76.10	2038.0
77.00	267.0
77.90	308.0
78.90	1522.0
80.00	455.0
80.90	1493.0
82.00	418.0
86.00	120.0
87.00	2185.0
88.00	2001.0
91.00	196.0
92.00	1331.0
93.10	2018.0
94.00	4980.0
95.10	41992.0
96.00	3024.0
103.90	202.0
105.90	210.0
110.90	108.0
115.90	166.0
116.90	330.0
117.90	275.0
118.90	334.0
128.00	196.0
129.90	164.0
131.00	130.0
135.00	147.0
136.90	150.0
140.80	478.0
142.00	128.0
143.00	629.0
144.90	179.0
145.90	108.0
154.90	127.0
156.90	106.0
171.00	212.0
172.00	586.0
174.00	36152.0
175.00	2794.0
176.00	35336.0
177.00	2524.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
36.00	547.0
37.10	2340.0
38.00	2051.0
39.10	1119.0
39.90	474.0
43.00	102.0
44.00	1498.0
45.00	368.0
46.00	193.0
47.10	763.0
47.90	406.0
49.00	1898.0
50.10	7743.0
51.00	2534.0
52.00	137.0
53.20	147.0
55.10	170.0
56.00	842.0
57.00	1170.0
58.00	222.0
60.00	500.0
61.00	1908.0
62.00	2385.0
63.10	1858.0
64.00	349.0
65.00	608.0
66.90	195.0
68.00	4133.0
69.00	4868.0
70.00	417.0
72.00	322.0
73.00	1828.0
74.00	6723.0
75.10	20856.0
76.10	1890.0
77.00	262.0
77.90	261.0
78.90	1413.0
79.90	456.0
80.90	1421.0
81.90	375.0
85.90	110.0
87.00	1850.0
88.00	1936.0
91.00	201.0
92.00	1098.0
93.00	2132.0
94.00	4884.0
95.00	40464.0
96.10	3036.0
103.90	178.0
105.10	111.0
105.80	183.0
110.90	125.0
115.90	192.0
116.90	256.0
117.90	300.0
118.90	328.0
128.00	172.0
130.00	145.0
131.00	127.0
135.00	138.0
137.00	123.0
140.90	448.0
142.00	105.0
143.00	488.0
144.90	191.0
145.90	128.0
154.90	146.0
170.90	229.0
172.00	621.0
174.00	35072.0
175.00	2806.0
176.00	34592.0
177.00	2445.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
36.10	105.0
40.00	449.0
40.80	119.0
44.00	1217.0
45.70	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60