

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022715.D
 Acq On : 08 Oct 2021 20:31
 Operator : SY/MD
 Sample : M4022-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B02

Quant Time: Oct 09 01:26:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:00:25 PM

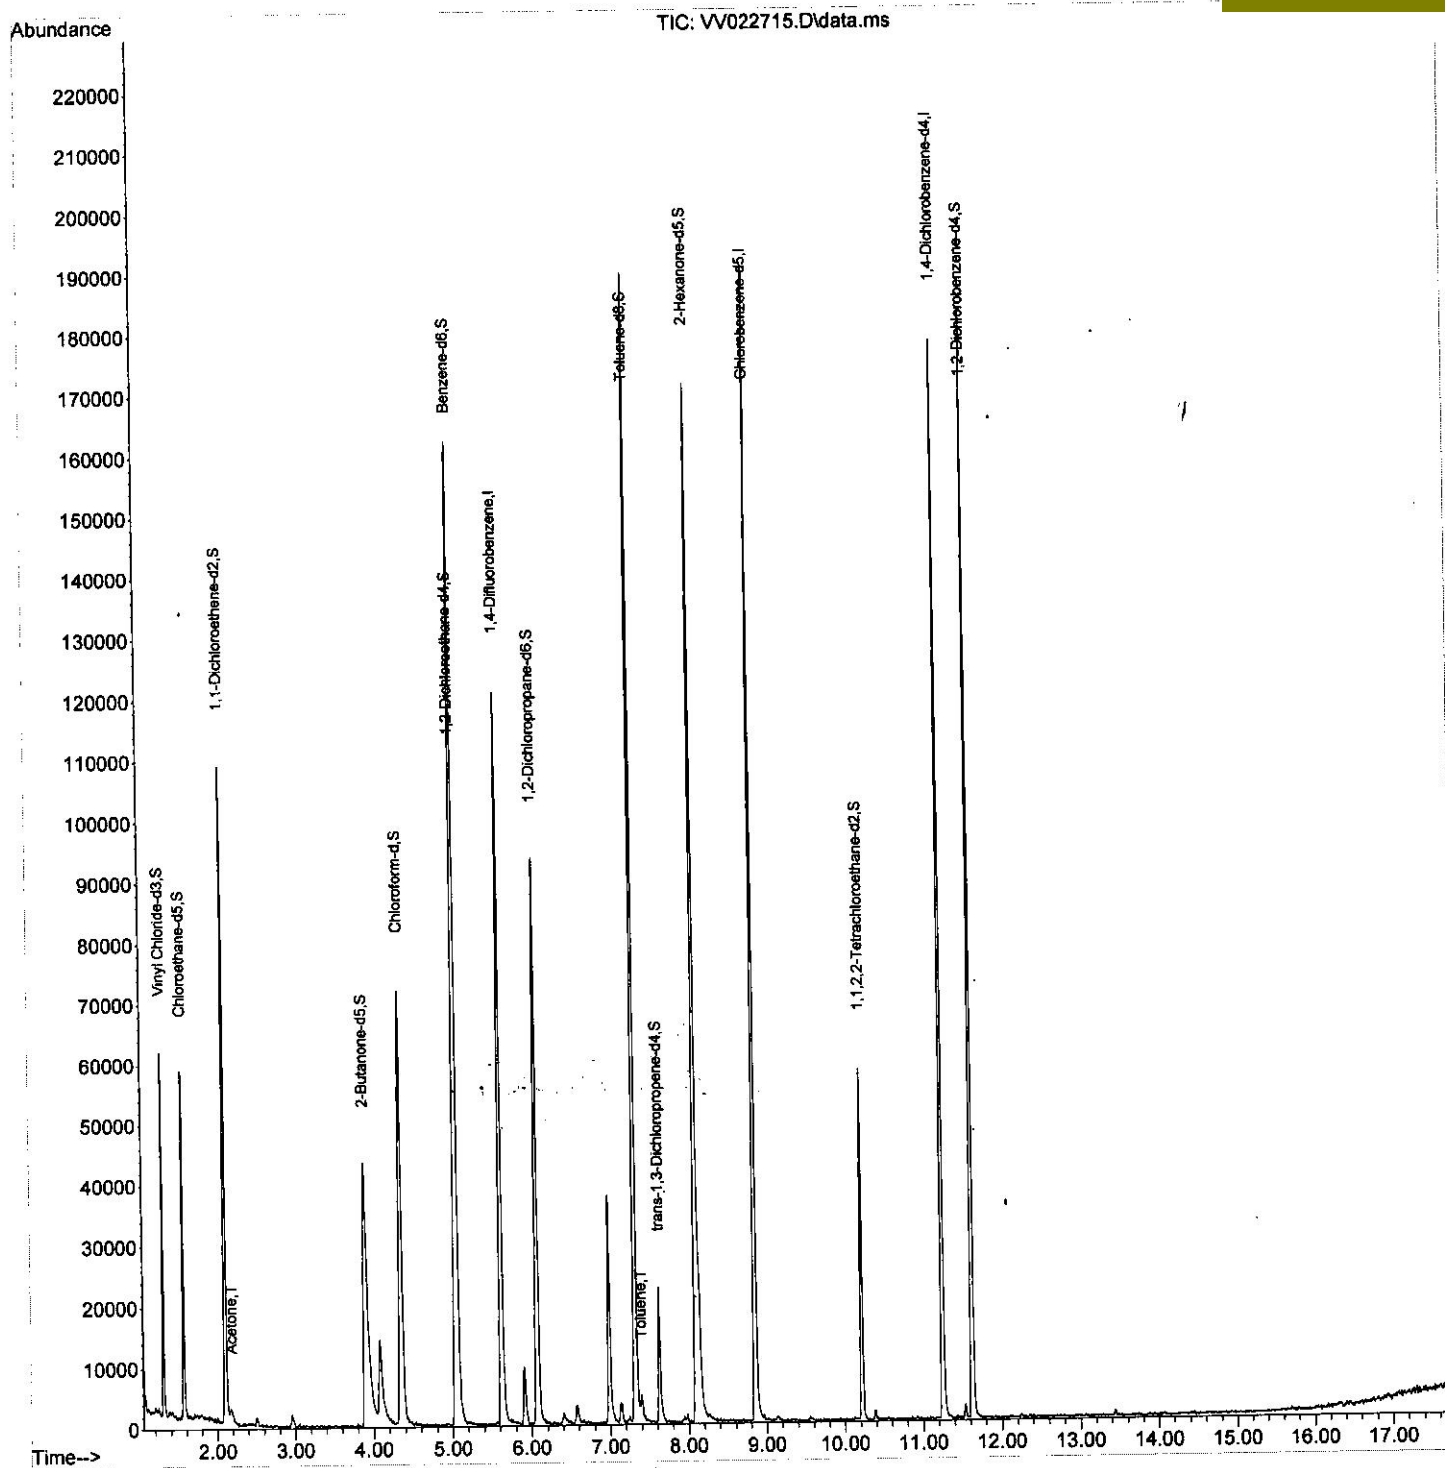

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022715.D
 Acq On : 08 Oct 2021 20:31
 Operator : SY/MD
 Sample : M4022-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B02

Quant Time: Oct 09 01:26:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:00:25 PM

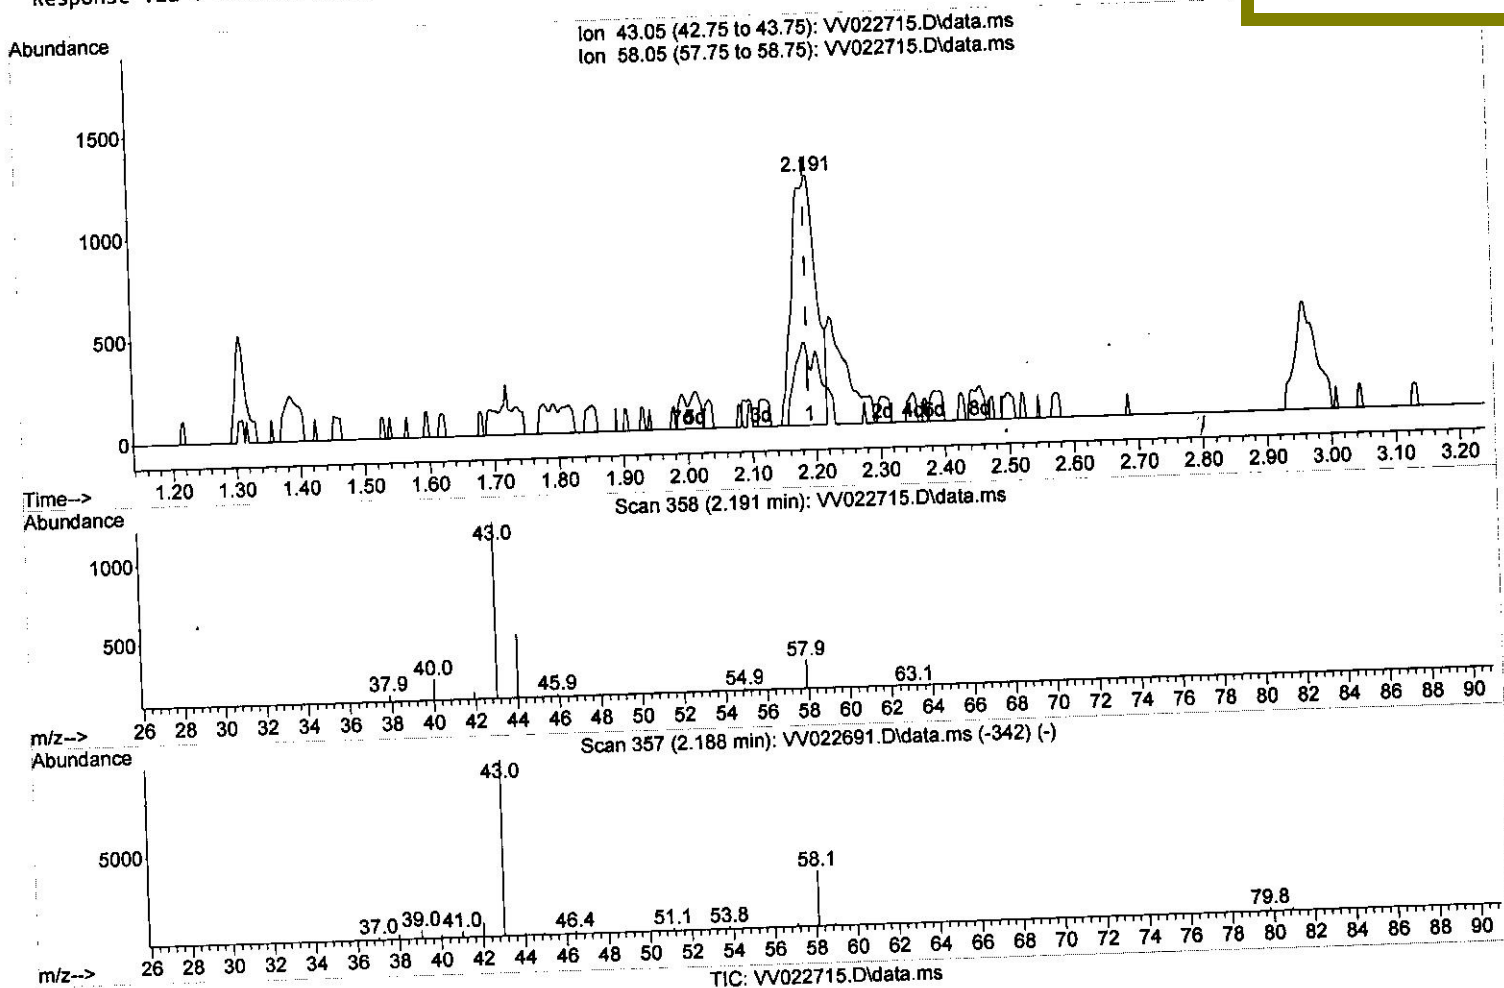

(13) Acetone (T)

2.191min (+ 0.003) 2.93 ug/L

response 3206

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	20.68
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022715.D
 Acq On : 08 Oct 2021 20:31
 Operator : SY/MD
 Sample : M4022-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B02

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:00:25 PM

Quant Time: Oct 09 01:26:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

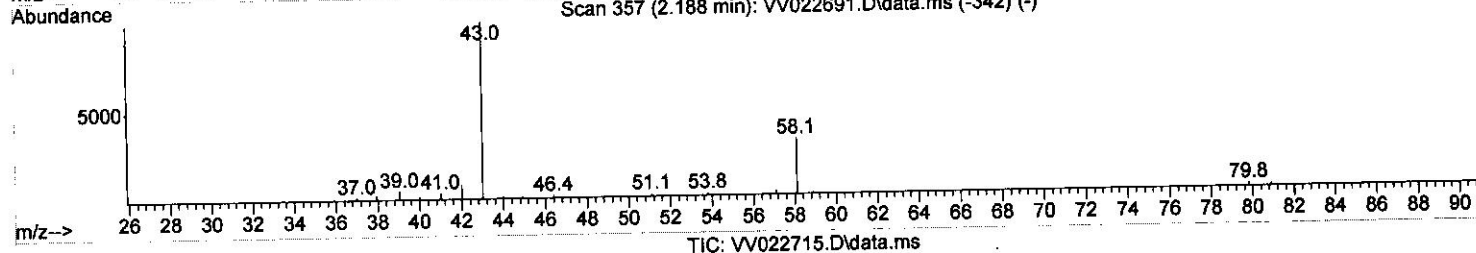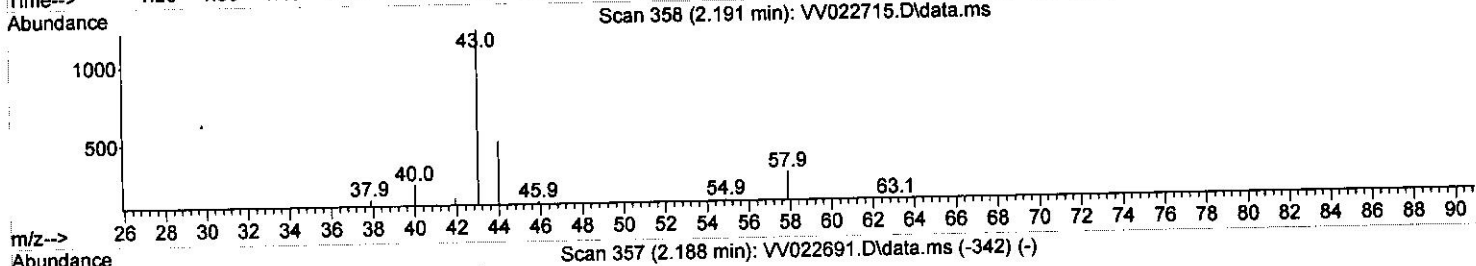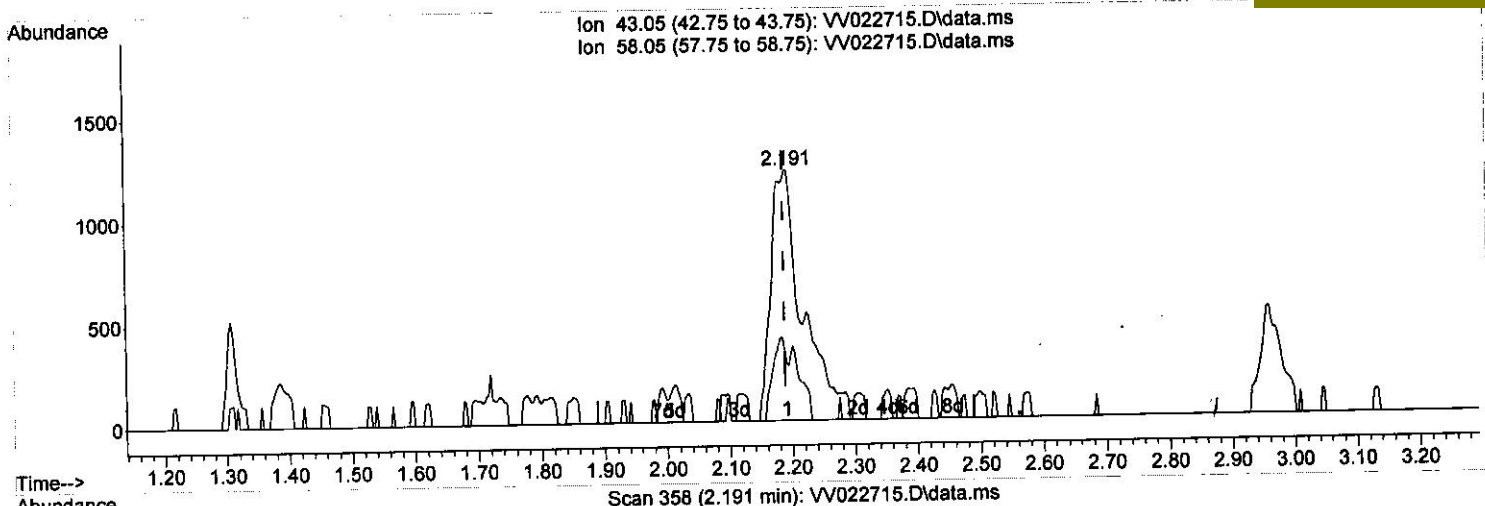

(13) Acetone (T)

2.191min (+ 0.003) 3.95 ug/L m

response 4328

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.10	15.32
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022715.D
 Acq On : 08 Oct 2021 20:31
 Operator : SY/MD
 Sample : M4022-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B02

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:00:25 PM

Quant Time: Oct 09 01:26:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	108932	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	112169	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	48780	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35272	4.706	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	94.200%		
7) Chloroethane-d5	1.568	69	35142	5.218	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	104.400%		
11) 1,1-Dichloroethene-d2	2.108	63	55802	3.796	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	76.000%		
20) 2-Butanone-d5	3.892	46	92204	46.920	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	93.840%		
24) Chloroform-d	4.349	84	75289	4.875	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.400%		
26) 1,2-Dichloroethane-d4	5.034	65	36835	4.914	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.200%		
32) Benzene-d6	5.053	84	149078	4.465	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.200%		
36) 1,2-Dichloropropane-d6	6.069	67	47641	4.818	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	96.400%		
41) Toluene-d8	7.317	98	126497	4.382	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	87.600%		
43) trans-1,3-Dichloroprop...	7.628	79	13699	4.176	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	83.600%		
46) 2-Hexanone-d5	8.091	63	52547	39.748	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	79.500%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	27618	4.123	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	82.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	49713	5.497	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	110.000%		
Target Compounds						
13) Acetone	2.191	43	4328m	3.950	ug/L	Qvalue
42) Toluene	7.400	91	3123	0.102	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 10/12/2021