

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022692.D
 Acq On : 08 Oct 2021 10:39
 Operator : SY/MD
 Sample : VV1008WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Quant Time: Oct 09 01:23:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	109109	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	110434	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	49256	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36014	4.798	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.000%
7) Chloroethane-d5	1.568	69	34513	5.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.400%
11) 1,1-Dichloroethene-d2	2.108	63	53863	3.658	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	3.908	46	53273	27.065	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	54.140%
24) Chloroform-d	4.349	84	72460	4.684	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
26) 1,2-Dichloroethane-d4	5.034	65	35914	4.783	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.600%
32) Benzene-d6	5.050	84	141967	4.318	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	6.072	67	45350	4.658	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.317	98	117319	4.128	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	7.625	79	13734	4.252	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.095	63	55594	42.714	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.420%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	29349	4.450	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	47444	5.195	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.000%
Target Compounds						
25) Chloroform	4.375	83	5246	0.351	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022692.D
Acq On : 08 Oct 2021 10:39
Operator : SY/MD
Sample : VV1008WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Time: Oct 09 01:23:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 09 01:23:25 2021
Response via : Initial Calibration

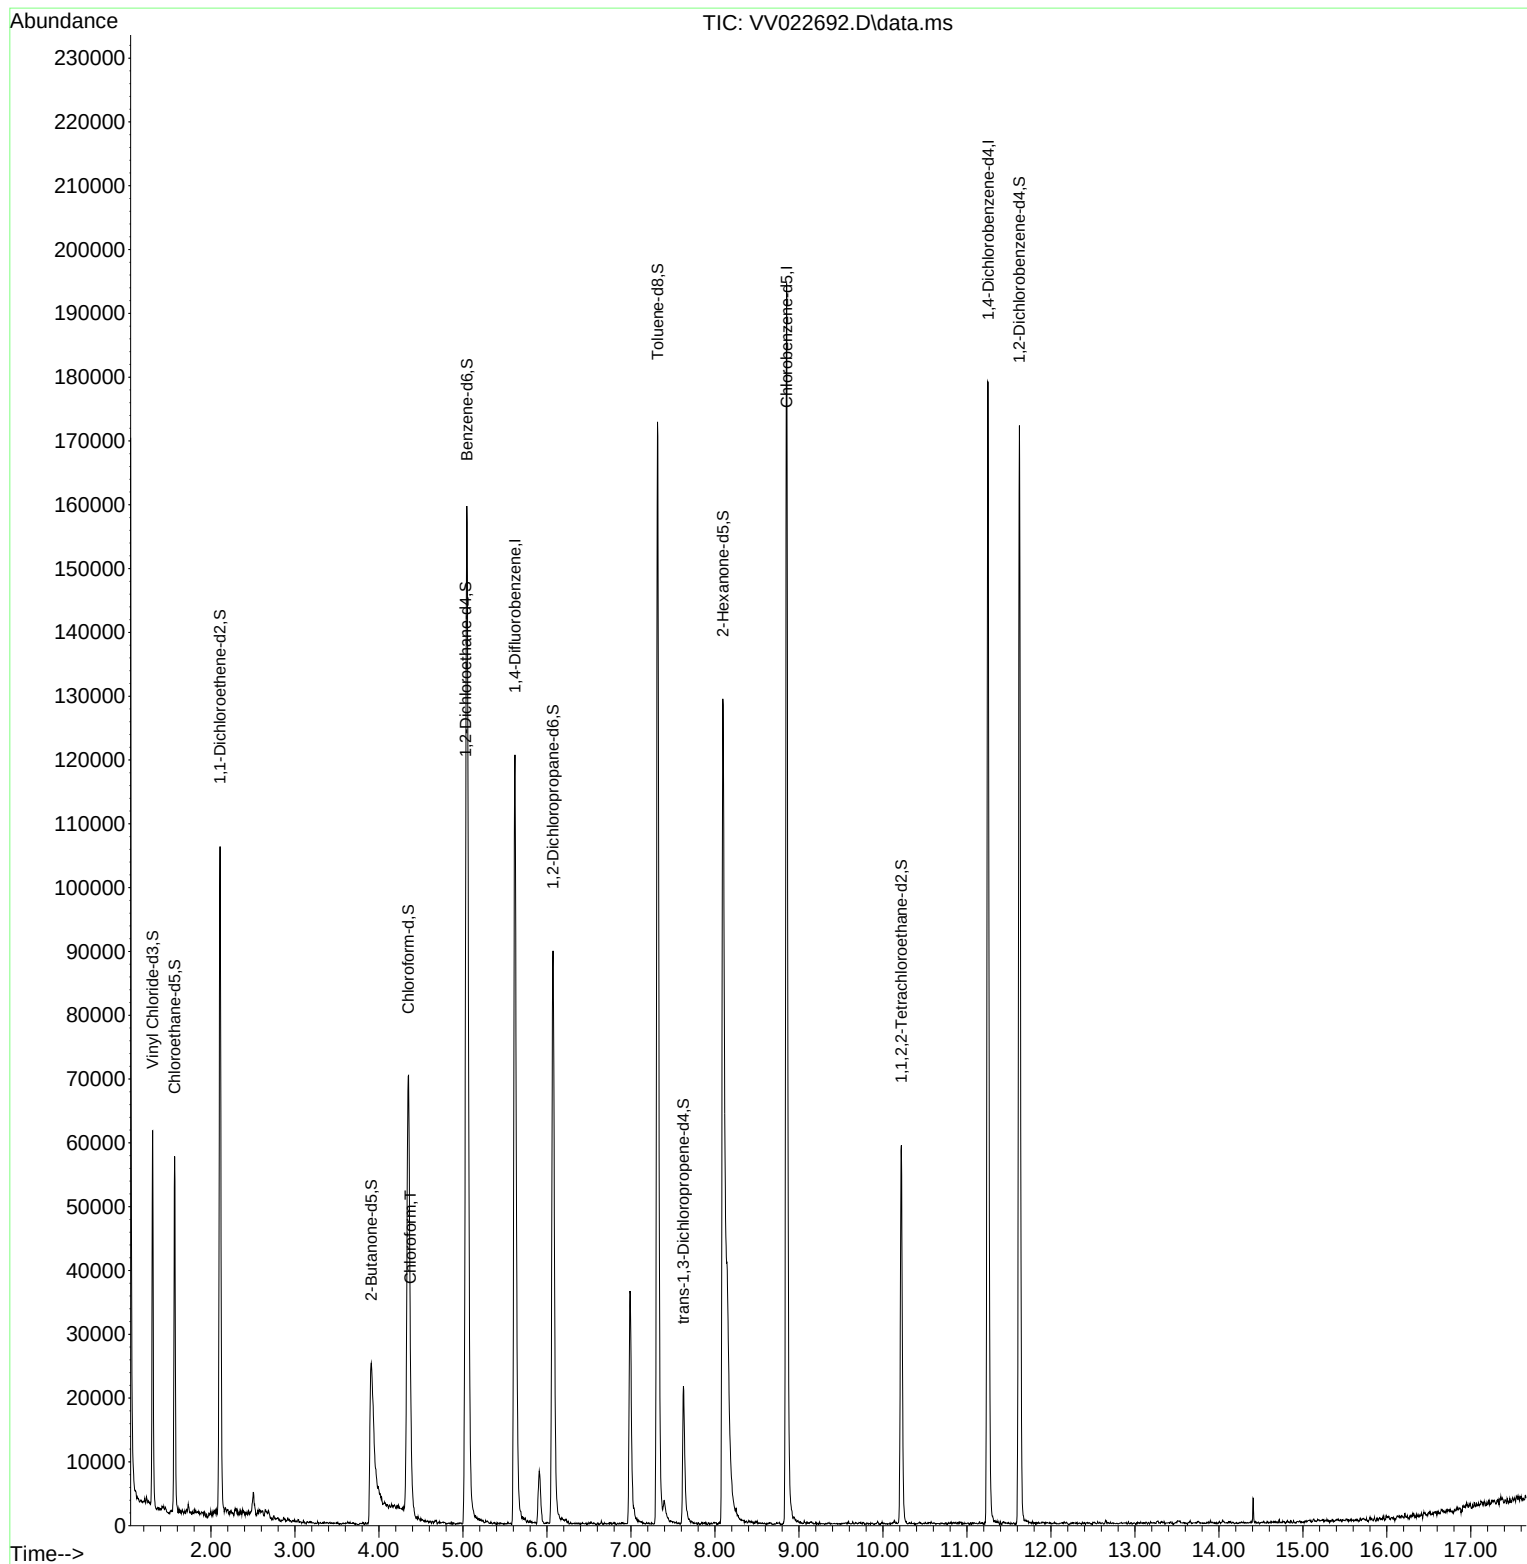

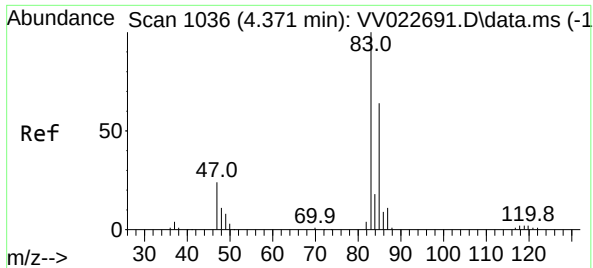

#25
Chloroform
Concen: 0.351 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. 0.003 min
Lab File: VV022692.D
Acq: 08 Oct 2021 10:39

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Tgt Ion: 83 Resp: 5246
Ion Ratio Lower Upper
83 100
85 63.7 45.7 84.9

