

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022696.D
 Acq On : 08 Oct 2021 12:33
 Operator : SY/MD
 Sample : M4027-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT6

Quant Time: Oct 09 01:24:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	108145	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	112400	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	50626	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	35825	4.815	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.200%
7) Chloroethane-d5	1.564	69	34805	5.205	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.200%
11) 1,1-Dichloroethene-d2	2.105	63	56501	3.871	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.400%
20) 2-Butanone-d5	3.908	46	72071	36.942	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	73.880%
24) Chloroform-d	4.349	84	74685	4.871	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	5.034	65	37812	5.081	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.053	84	148759	4.446	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	6.072	67	47004	4.743	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.317	98	127239	4.399	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	7.628	79	14315	4.355	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.095	63	58845	44.421	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.840%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	29937	4.460	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	50708	5.402	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.000%
Target Compounds						Qvalue
3) Chloromethane	1.240	50	2477	0.313	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022696.D
Acq On : 08 Oct 2021 12:33
Operator : SY/MD
Sample : M4027-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Time: Oct 09 01:24:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 09 01:23:25 2021
Response via : Initial Calibration

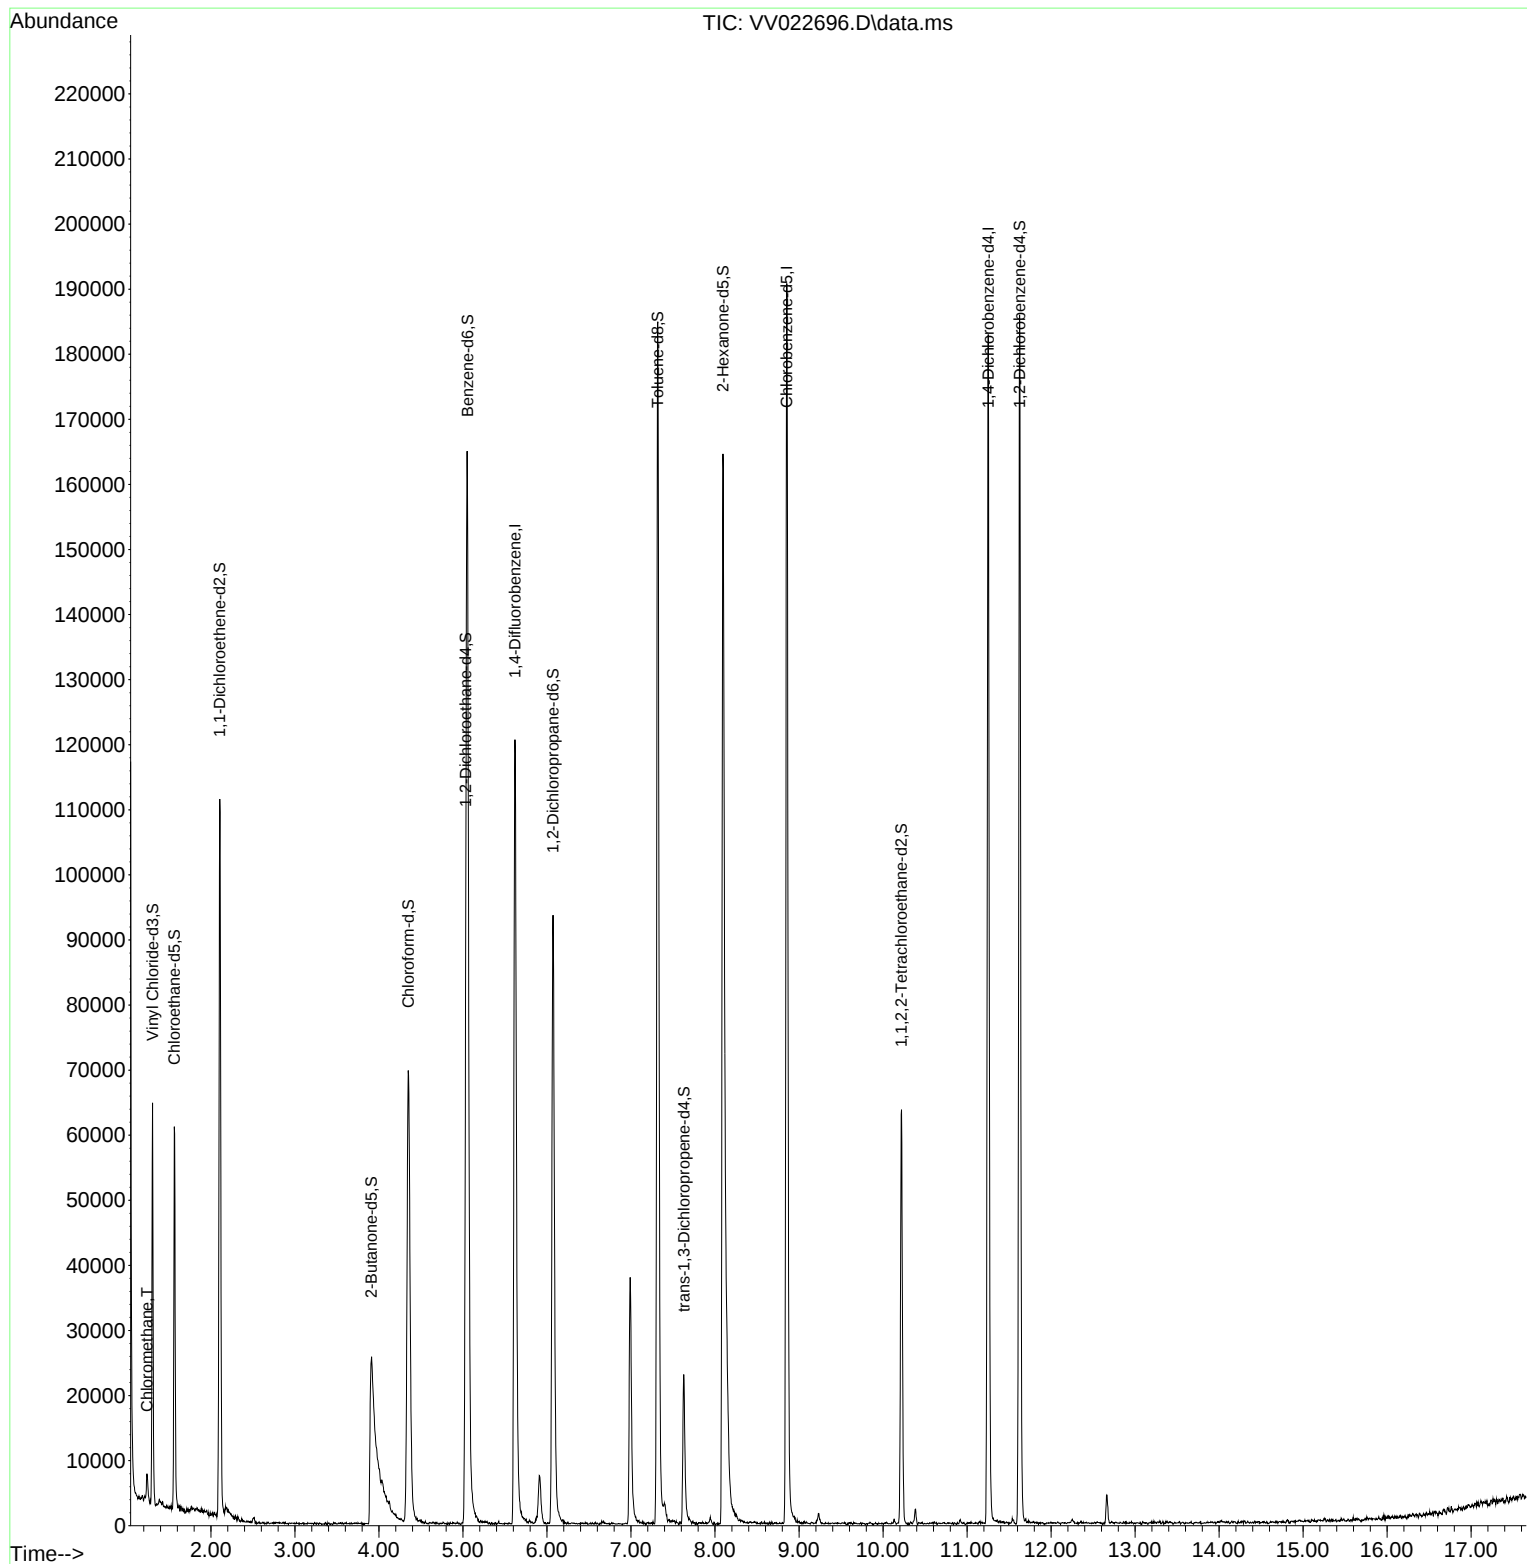

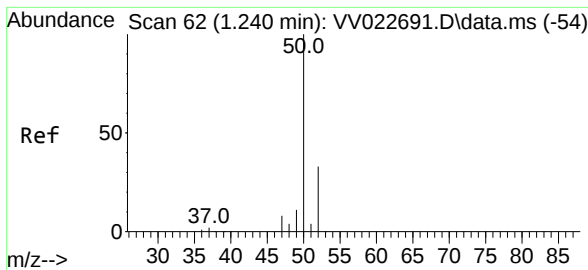

#3
 Chloromethane
 Concen: 0.313 ug/L
 RT: 1.240 min Scan# 62
 Delta R.T. -0.000 min
 Lab File: VV022696.D
 Acq: 08 Oct 2021 12:33

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT6

Tgt Ion: 50 Resp: 2477
 Ion Ratio Lower Upper
 50 100
 52 34.4 22.9 42.5

