

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022704.D
 Acq On : 08 Oct 2021 15:44
 Operator : SY/MD
 Sample : M4098-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT21

Quant Time: Oct 09 01:25:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 09 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	103566	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	106086	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	47787	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36676	5.147	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.000%
7) Chloroethane-d5	1.568	69	36008	5.623	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.400%
11) 1,1-Dichloroethene-d2	2.108	63	56655	4.053	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.000%
20) 2-Butanone-d5	3.896	46	94029	50.328	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.660%
24) Chloroform-d	4.352	84	76390	5.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.000%
26) 1,2-Dichloroethane-d4	5.037	65	37200	5.220	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.400%
32) Benzene-d6	5.053	84	152255	4.821	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
36) 1,2-Dichloropropane-d6	6.072	67	47550	5.084	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.600%
41) Toluene-d8	7.320	98	126269	4.625	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%
43) trans-1,3-Dichloroprop...	7.625	79	14028	4.521	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.091	63	56731	45.374	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.740%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32392	5.113	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	52105	5.881	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.600%
Target Compounds						Qvalue
13) Acetone	2.179	43	2134	2.048	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022704.D
Acq On : 08 Oct 2021 15:44
Operator : SY/MD
Sample : M4098-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT21


Quant Time: Oct 09 01:25:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 09 01:23:25 2021
Response via : Initial Calibration

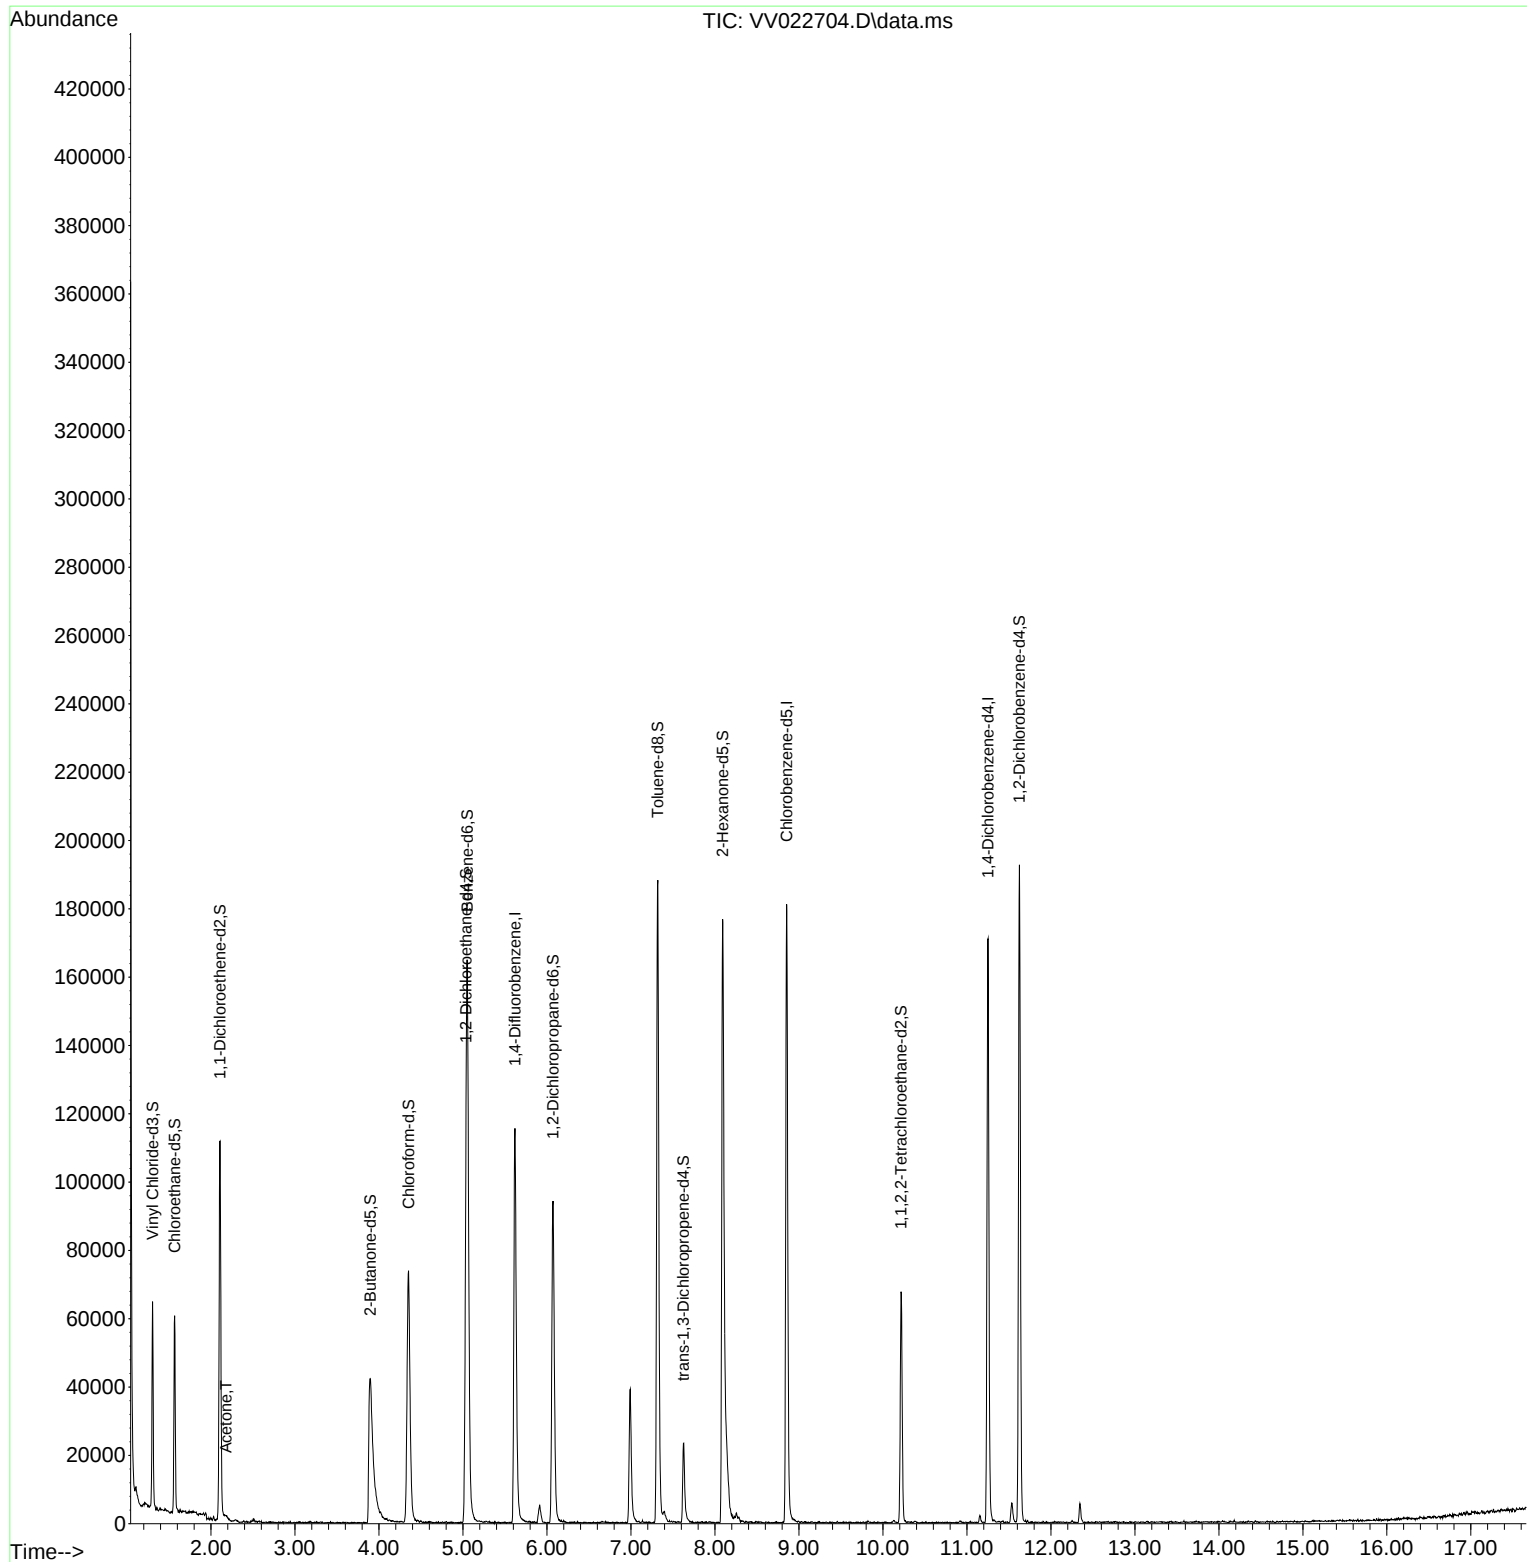

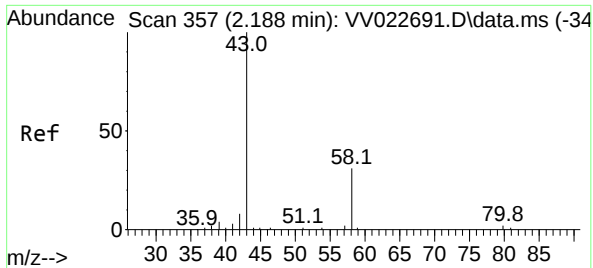

#13
 Acetone
 Concen: 2.048 ug/L
 RT: 2.179 min Scan# 354
 Delta R.T. -0.010 min
 Lab File: VV022704.D
 Acq: 08 Oct 2021 15:44

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT21

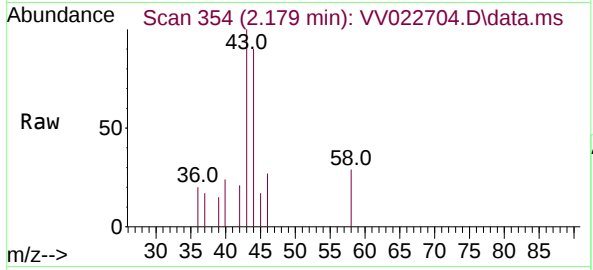

Tgt Ion:	43	Resp:	2134
Ion	Ratio	Lower	Upper
43	100		
58	14.4	0.0	24.2

