

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022694.D
 Acq On : 08 Oct 2021 11:45
 Operator : SY/MD
 Sample : M4027-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	92	rBV	57701	58423	15.34%	1.862%
2	1.568	155	164	173	rBV	55510	62319	16.36%	1.986%
3	2.105	322	331	345	rBV	99647	141298	37.09%	4.502%
4	2.503	447	455	464	rVB4	2960	4584	1.20%	0.146%
5	3.921	880	896	928	rBV2	27633	111340	29.23%	3.548%
6	4.349	1013	1029	1053	rVB	68896	170688	44.80%	5.439%
7	5.047	1230	1246	1268	rBV2	160617	380962	100.00%	12.139%
8	5.619	1411	1424	1445	rBV	132141	266527	69.96%	8.492%
9	5.902	1502	1512	1524	rBV3	10647	22116	5.81%	0.705%
10	6.072	1551	1565	1585	rBV	86991	179867	47.21%	5.731%
11	6.992	1836	1851	1871	rBV	35686	67281	17.66%	2.144%
12	7.317	1939	1952	1971	rBV	162392	291181	76.43%	9.278%
13	7.400	1971	1978	1989	rVB3	3648	7290	1.91%	0.232%
14	7.625	2039	2048	2067	rBV2	20794	37738	9.91%	1.202%
15	8.101	2184	2196	2238	rBV3	120831	358439	94.09%	11.421%
16	8.853	2417	2430	2459	rBV	201987	335863	88.16%	10.702%
17	10.220	2842	2855	2867	rBV	51973	83863	22.01%	2.672%
18	11.249	3162	3175	3202	rBV	187233	297117	77.99%	9.467%
19	11.625	3281	3292	3312	rBV	168904	261562	68.66%	8.334%




Sum of corrected areas: 3138458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022694.D
Acq On : 08 Oct 2021 11:45
Operator : SY/MD
Sample : M4027-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

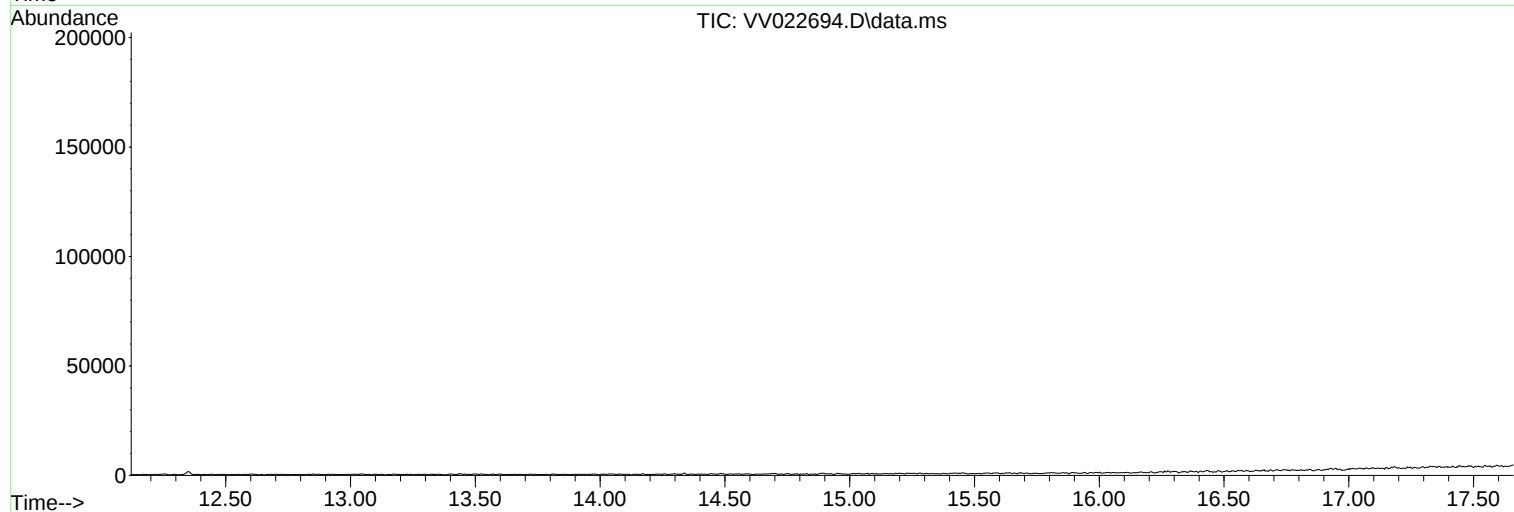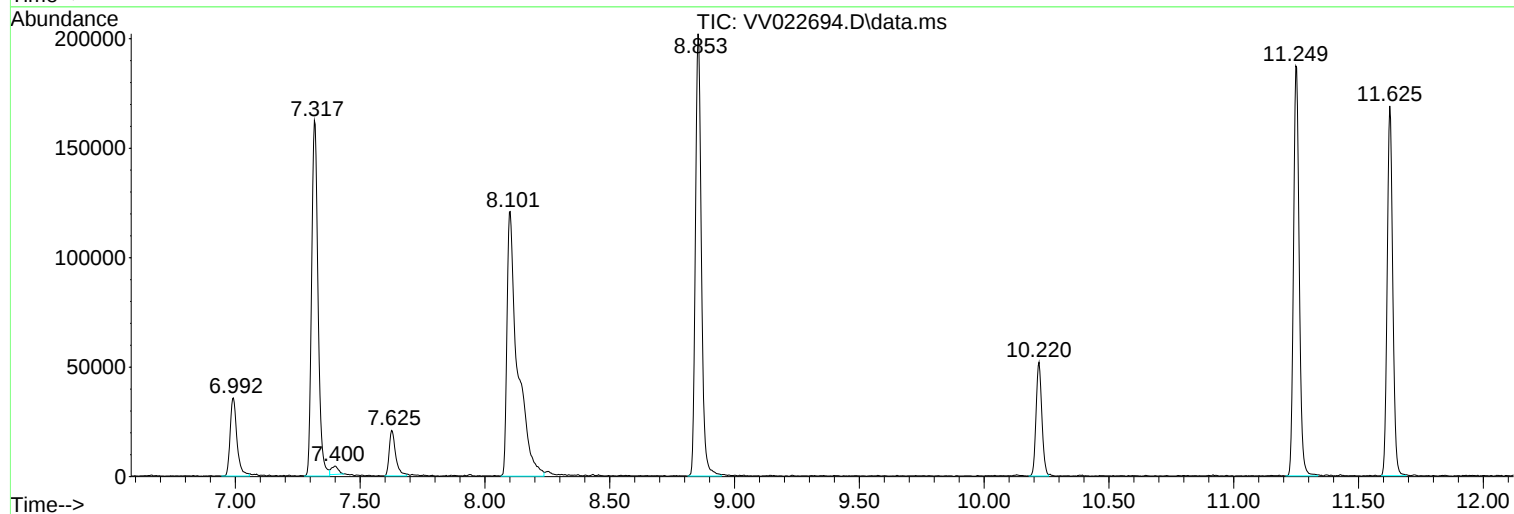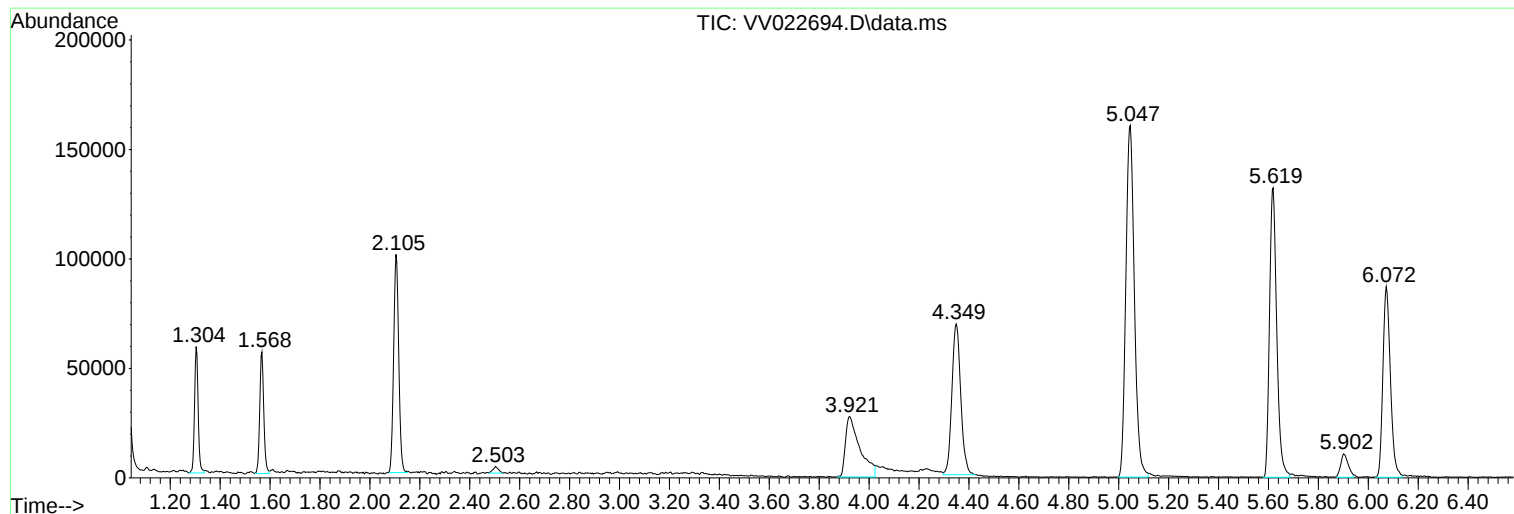

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022694.D
Acq On : 08 Oct 2021 11:45
Operator : SY/MD
Sample : M4027-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022694.D
Acq On : 08 Oct 2021 11:45
Operator : SY/MD
Sample : M4027-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
