

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022696.D
 Acq On : 08 Oct 2021 12:33
 Operator : SY/MD
 Sample : M4027-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	72	rVB	4508	6117	1.50%	0.185%
2	1.304	75	82	93	rVB	61886	60262	14.80%	1.827%
3	1.564	155	163	177	rBV	58758	66544	16.34%	2.018%
4	2.105	320	331	346	rBV	110315	160581	39.44%	4.870%
5	3.912	881	893	921	rBV2	25705	111777	27.45%	3.390%
6	4.349	1012	1029	1054	rBV	69248	178098	43.74%	5.401%
7	5.050	1231	1247	1279	rBV3	164685	407137	100.00%	12.346%
8	5.619	1411	1424	1447	rBV	120508	248221	60.97%	7.527%
9	5.908	1506	1514	1532	rVB4	7342	16320	4.01%	0.495%
10	6.072	1551	1565	1596	rBV	93477	195568	48.03%	5.931%
11	6.989	1839	1850	1876	rBV	37891	72567	17.82%	2.201%
12	7.320	1941	1953	1974	rBV	184722	330792	81.25%	10.031%
13	7.628	2040	2049	2067	rBV2	22913	41680	10.24%	1.264%
14	8.095	2184	2194	2233	rBV3	164362	397062	97.53%	12.041%
15	8.853	2417	2430	2454	rBV	190555	319400	78.45%	9.686%
16	10.220	2844	2855	2873	rVB	63631	100050	24.57%	3.034%
17	11.252	3165	3176	3194	rBV	182725	284025	69.76%	8.613%
18	11.625	3278	3292	3310	rBV	185841	294882	72.43%	8.942%
19	12.664	3608	3615	3626	rVB4	4377	6578	1.62%	0.199%




Sum of corrected areas: 3297661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022696.D
Acq On : 08 Oct 2021 12:33
Operator : SY/MD
Sample : M4027-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

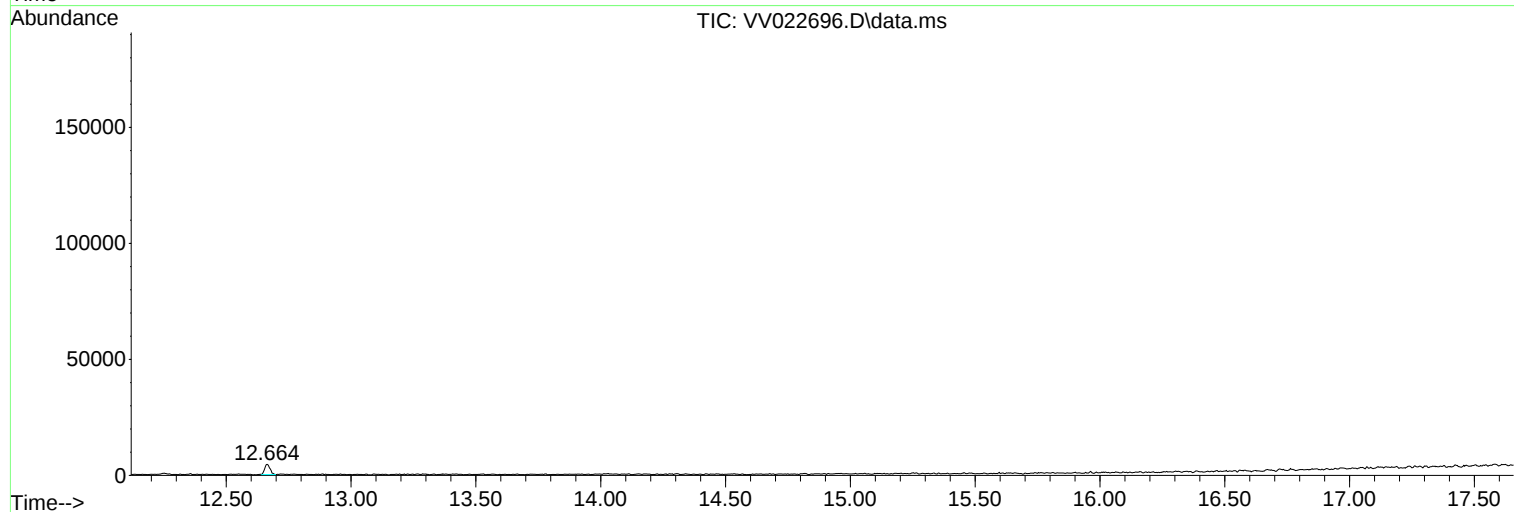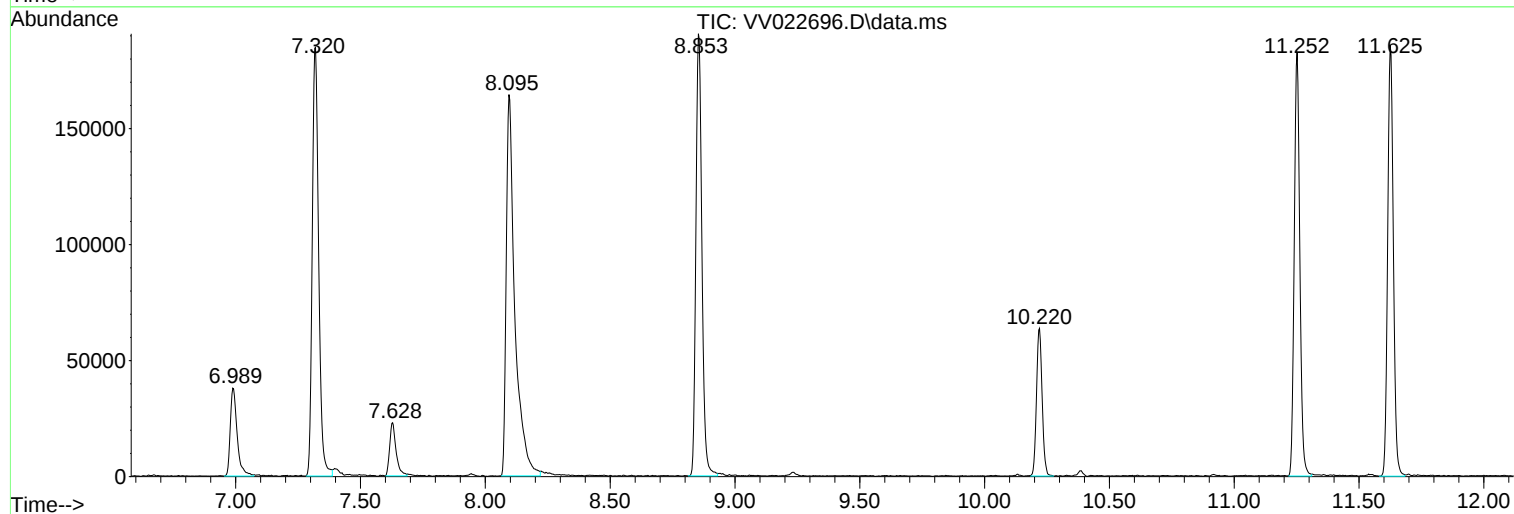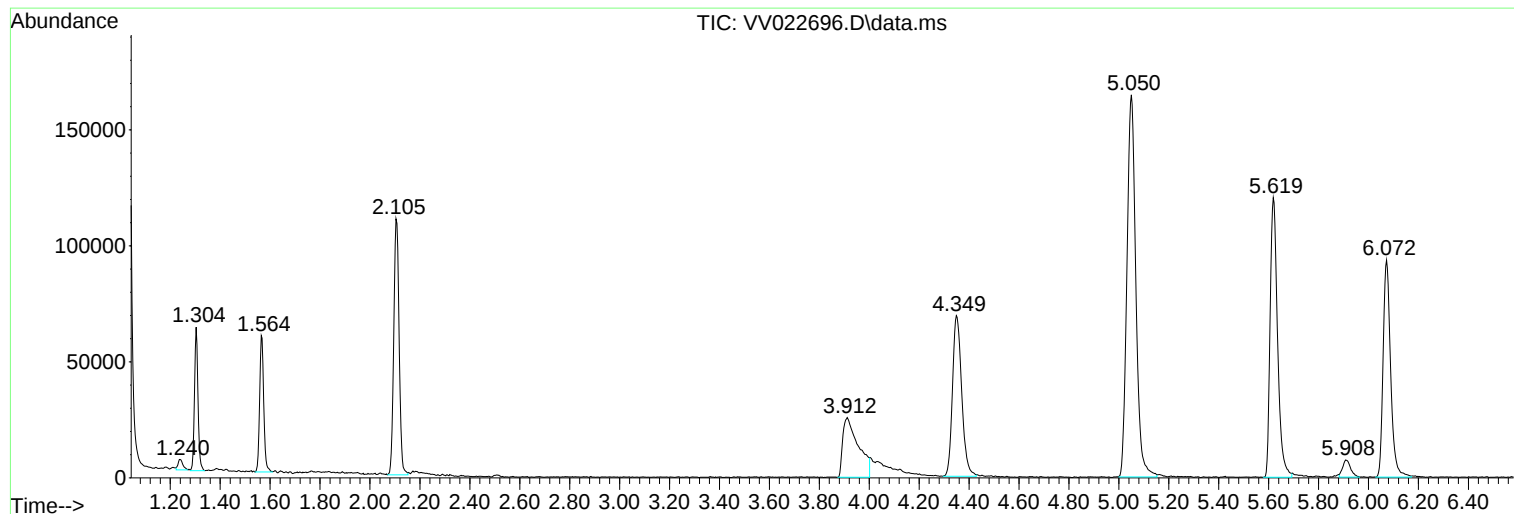

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022696.D
Acq On : 08 Oct 2021 12:33
Operator : SY/MD
Sample : M4027-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022696.D
Acq On : 08 Oct 2021 12:33
Operator : SY/MD
Sample : M4027-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
