

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022697.D
 Acq On : 08 Oct 2021 12:56
 Operator : SY/MD
 Sample : M4051-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	62716	64065	14.93%	1.858%
2	1.568	156	164	178	rBV	59675	67419	15.71%	1.956%
3	2.104	321	331	344	rBV	109495	156197	36.40%	4.531%
4	2.503	444	455	470	rVB2	13656	24661	5.75%	0.715%
5	3.918	881	895	917	rBV2	31985	113761	26.51%	3.300%
6	4.349	1013	1029	1049	rVB	78597	193723	45.15%	5.619%
7	5.043	1225	1245	1268	rBV2	183153	429103	100.00%	12.447%
8	5.619	1410	1424	1453	rBV	129878	265484	61.87%	7.701%
9	5.905	1502	1513	1525	rBV3	8739	18377	4.28%	0.533%
10	6.072	1550	1565	1588	rBV2	99422	203299	47.38%	5.897%
11	6.989	1840	1850	1871	rBV2	41285	76466	17.82%	2.218%
12	7.316	1941	1952	1969	rBV	190960	328706	76.60%	9.535%
13	7.394	1972	1976	1995	rVB6	3292	6444	1.50%	0.187%
14	7.625	2039	2048	2067	rBV	23136	43900	10.23%	1.273%
15	8.098	2181	2195	2234	rBV2	148602	419403	97.74%	12.166%
16	8.853	2419	2430	2461	rBV	204161	333748	77.78%	9.681%
17	10.220	2841	2855	2869	rBV	64497	105327	24.55%	3.055%
18	11.252	3165	3176	3200	rBV	188201	295983	68.98%	8.586%
19	11.625	3281	3292	3313	rBV	191109	301299	70.22%	8.740%




Sum of corrected areas: 3447365

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022697.D
Acq On : 08 Oct 2021 12:56
Operator : SY/MD
Sample : M4051-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

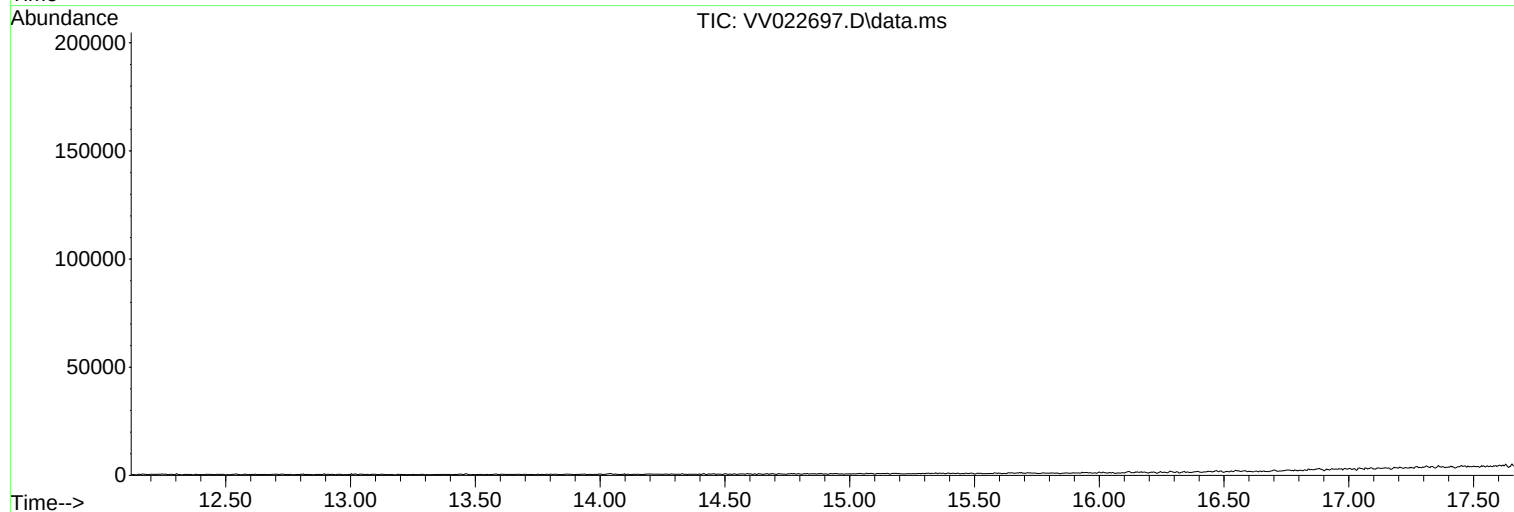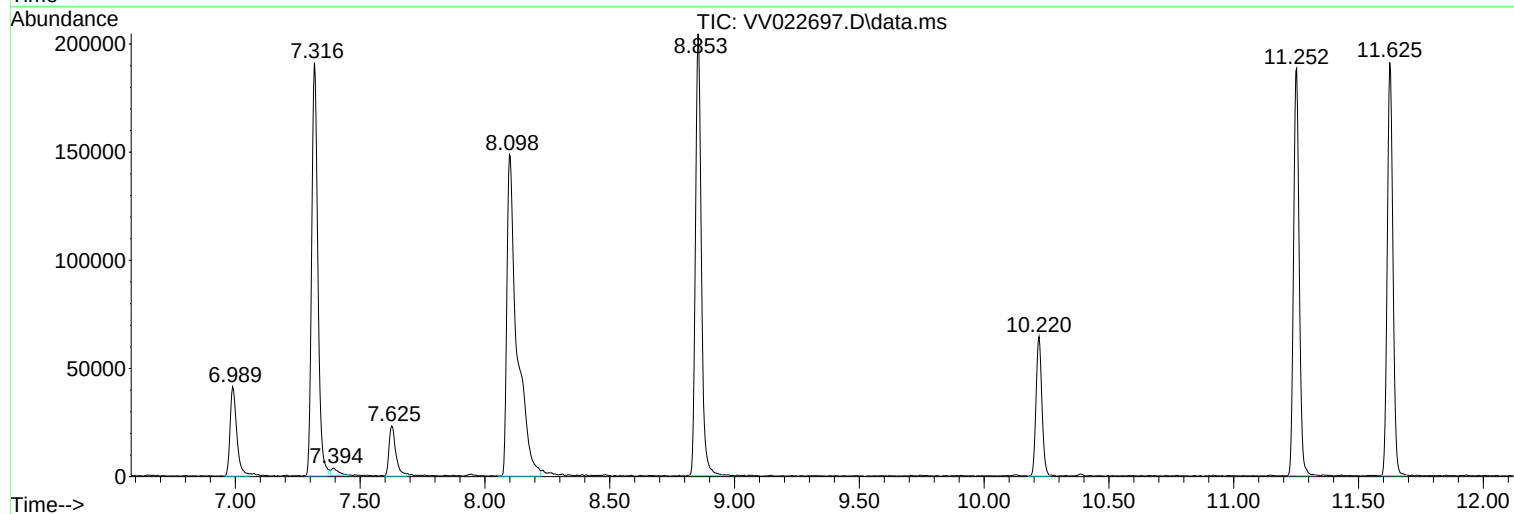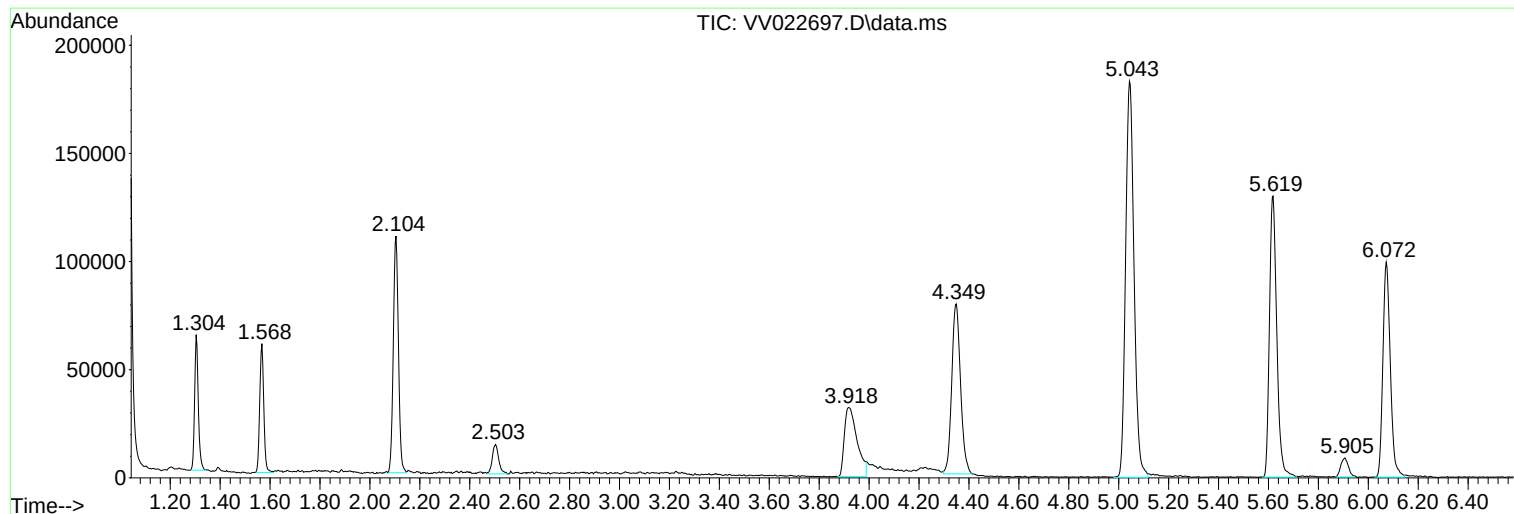

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022697.D
Acq On : 08 Oct 2021 12:56
Operator : SY/MD
Sample : M4051-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022697.D
Acq On : 08 Oct 2021 12:56
Operator : SY/MD
Sample : M4051-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
