

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022698.D
 Acq On : 08 Oct 2021 13:20
 Operator : SY/MD
 Sample : M4052-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	61823	61677	15.67%	1.909%
2	1.568	155	164	173	rBV	58915	64759	16.46%	2.004%
3	2.105	320	331	343	rBV	102567	149296	37.94%	4.620%
4	2.503	445	455	467	rBV	21267	35043	8.90%	1.085%
5	3.912	883	893	916	rBV	29920	100819	25.62%	3.120%
6	4.349	1013	1029	1052	rVB2	71097	182001	46.25%	5.633%
7	5.044	1230	1245	1265	rBV2	164979	393550	100.00%	12.179%
8	5.619	1411	1424	1446	rBV	125094	253688	64.46%	7.851%
9	5.908	1502	1514	1528	rBV2	8643	17542	4.46%	0.543%
10	6.072	1550	1565	1585	rBV2	92518	192530	48.92%	5.958%
11	6.989	1839	1850	1871	rBV2	37900	70112	17.82%	2.170%
12	7.317	1941	1952	1971	rBV	173984	306212	77.81%	9.477%
13	7.394	1971	1976	1991	rVB5	3330	6483	1.65%	0.201%
14	7.629	2038	2049	2067	rBV2	22735	41696	10.59%	1.290%
15	8.098	2185	2195	2229	rBV3	141671	380289	96.63%	11.769%
16	8.854	2419	2430	2452	rBV	193275	317224	80.61%	9.817%
17	10.220	2843	2855	2871	rBV	62147	97233	24.71%	3.009%
18	11.252	3162	3176	3195	rBV	179973	283180	71.96%	8.764%
19	11.625	3280	3292	3315	rBV	173071	277923	70.62%	8.601%




Sum of corrected areas: 3231257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022698.D
Acq On : 08 Oct 2021 13:20
Operator : SY/MD
Sample : M4052-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

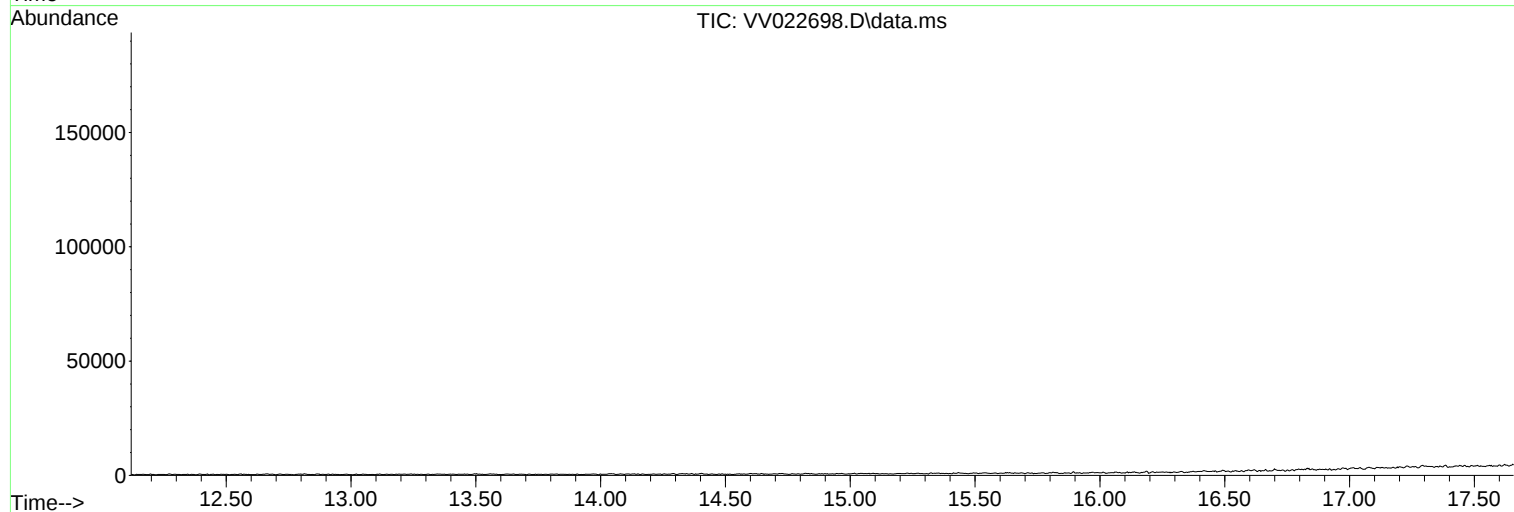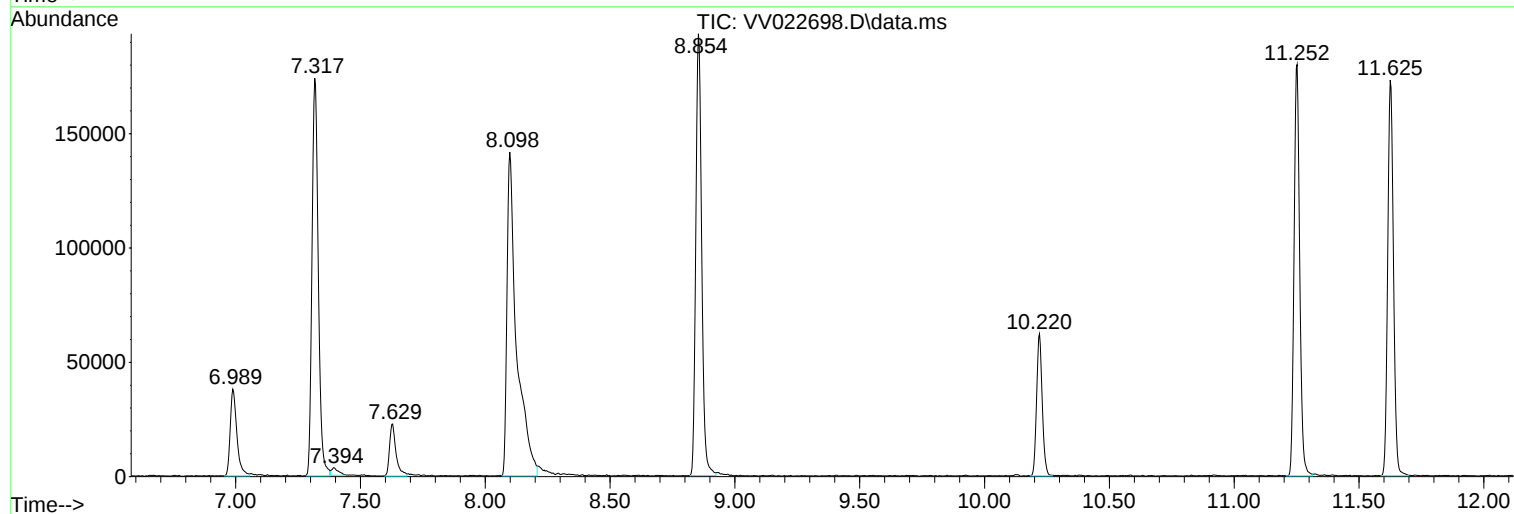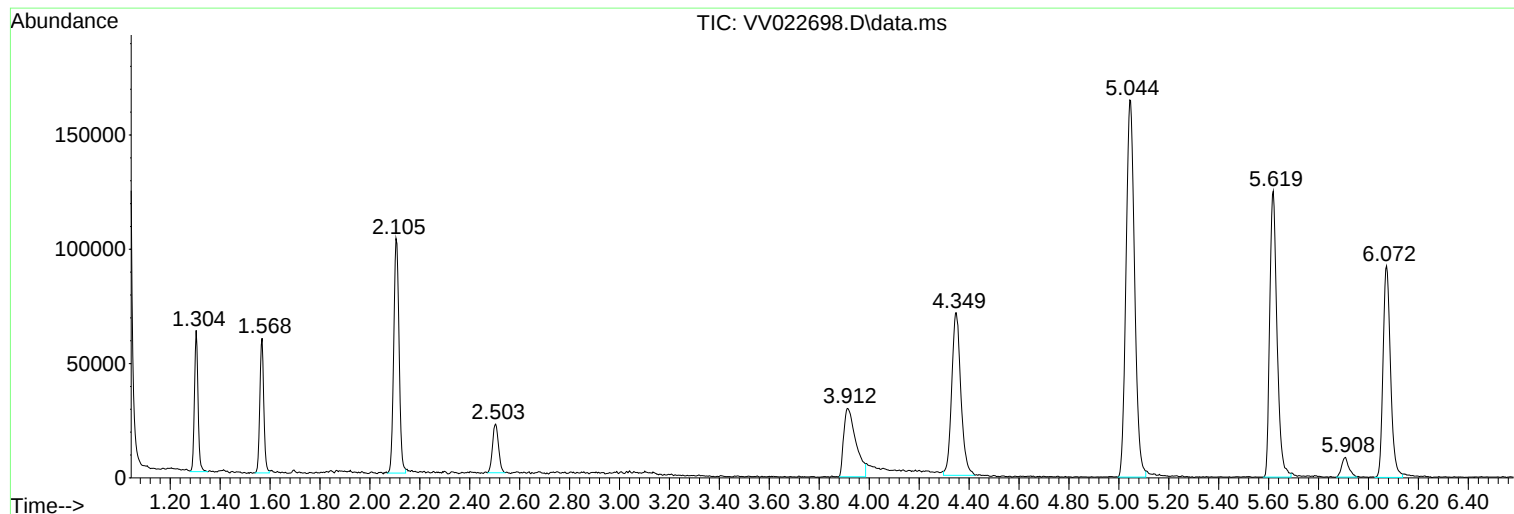

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022698.D
Acq On : 08 Oct 2021 13:20
Operator : SY/MD
Sample : M4052-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022698.D
Acq On : 08 Oct 2021 13:20
Operator : SY/MD
Sample : M4052-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
