

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022699.D
 Acq On : 08 Oct 2021 13:44
 Operator : SY/MD
 Sample : M4098-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT59

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	92	rBV	59776	60472	14.32%	1.776%
2	1.565	155	163	174	rBV	59392	66114	15.66%	1.942%
3	2.102	320	330	344	rBV	107847	155365	36.80%	4.563%
4	3.925	881	897	923	rBV	28792	115227	27.30%	3.385%
5	4.346	1013	1028	1060	rVB	80528	216718	51.34%	6.366%
6	5.044	1229	1245	1269	rBV2	180304	422148	100.00%	12.400%
7	5.616	1411	1423	1448	rBV	133962	272654	64.59%	8.009%
8	5.905	1502	1513	1530	rVB5	10898	23211	5.50%	0.682%
9	6.072	1550	1565	1592	rBV	98656	201435	47.72%	5.917%
10	6.989	1841	1850	1866	rBV	38792	71021	16.82%	2.086%
11	7.317	1941	1952	1970	rBV	187360	329162	77.97%	9.668%
12	7.397	1971	1977	1996	rVB5	3920	8845	2.10%	0.260%
13	7.625	2038	2048	2065	rBV	23017	42188	9.99%	1.239%
14	8.101	2184	2196	2234	rBV3	134680	386776	91.62%	11.361%
15	8.854	2419	2430	2455	rBV	207159	339115	80.33%	9.961%
16	10.220	2843	2855	2873	rBV	55937	91272	21.62%	2.681%
17	11.252	3162	3176	3191	rBV	192827	299231	70.88%	8.789%
18	11.535	3255	3264	3281	rBV6	4166	9623	2.28%	0.283%
19	11.625	3281	3292	3309	rBV	186771	293959	69.63%	8.634%




Sum of corrected areas: 3404536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022699.D
Acq On : 08 Oct 2021 13:44
Operator : SY/MD
Sample : M4098-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

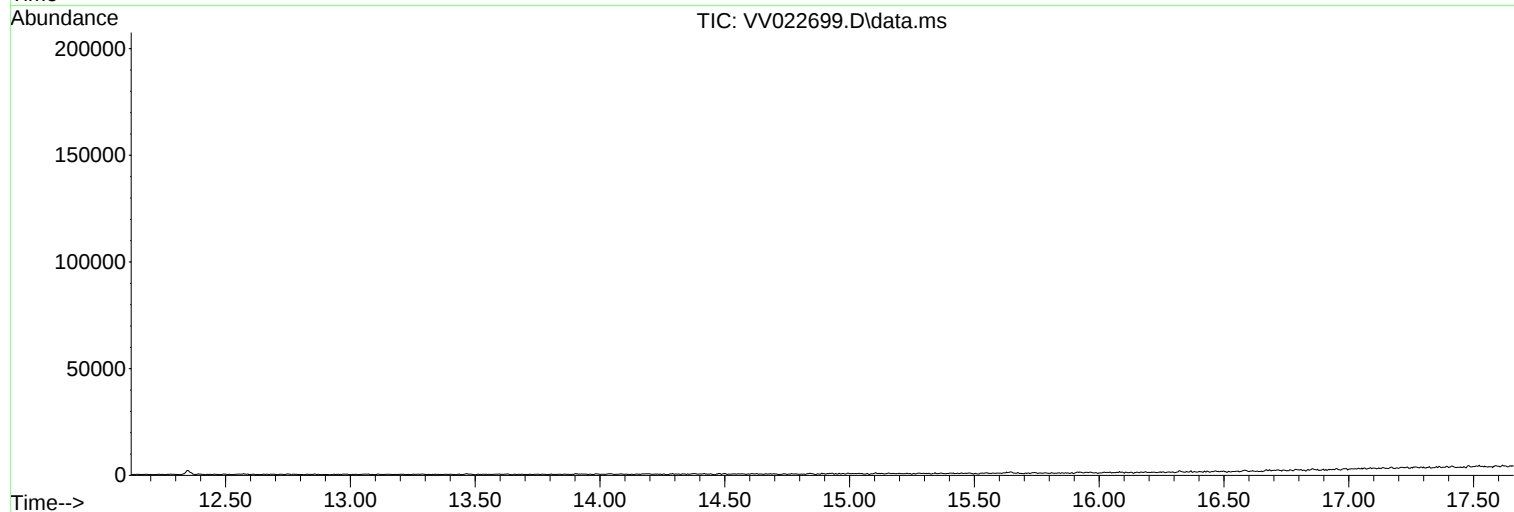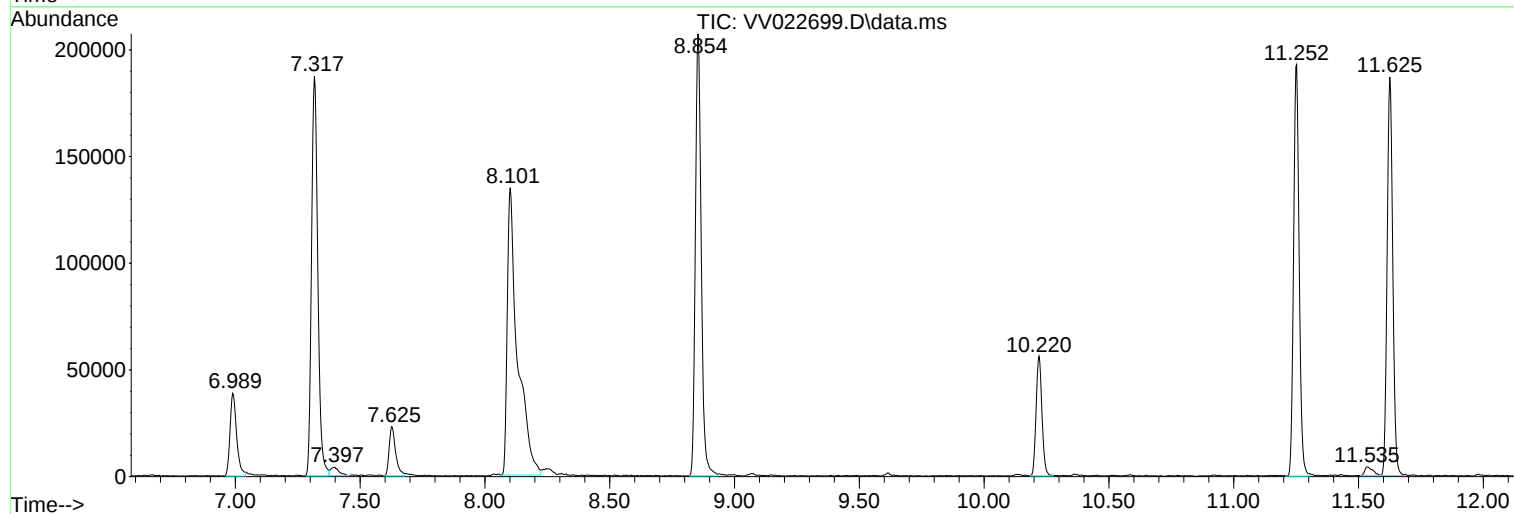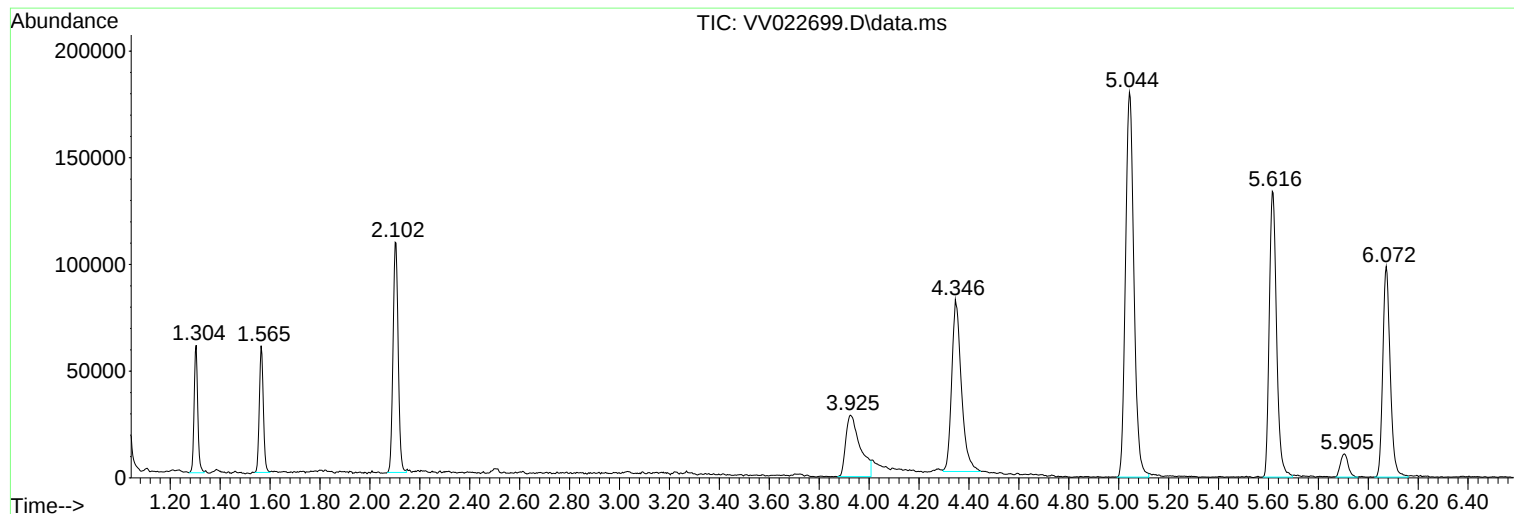

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022699.D
Acq On : 08 Oct 2021 13:44
Operator : SY/MD
Sample : M4098-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022699.D
Acq On : 08 Oct 2021 13:44
Operator : SY/MD
Sample : M4098-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
