

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022704.D
 Acq On : 08 Oct 2021 15:44
 Operator : SY/MD
 Sample : M4098-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	61070	64575	15.60%	1.937%
2	1.568	155	164	177	rBV	57795	67592	16.32%	2.028%
3	2.108	319	332	347	rBV	110881	164353	39.69%	4.931%
4	3.896	876	888	924	rBV2	42226	156361	37.76%	4.691%
5	4.352	1012	1030	1055	rBV	73609	183857	44.40%	5.516%
6	5.050	1230	1247	1276	rBV2	164821	414054	100.00%	12.422%
7	5.619	1412	1424	1450	rBV	115463	236135	57.03%	7.085%
8	5.915	1506	1516	1527	rBV5	5004	10033	2.42%	0.301%
9	6.072	1551	1565	1588	rBV	94181	197439	47.68%	5.924%
10	6.992	1837	1851	1869	rBV2	39315	72878	17.60%	2.186%
11	7.320	1941	1953	1971	rBV	188045	330002	79.70%	9.901%
12	7.397	1972	1977	1992	rVB6	3062	6088	1.47%	0.183%
13	7.628	2037	2049	2071	rBV2	23197	40516	9.79%	1.216%
14	8.091	2183	2193	2226	rBV2	176657	390642	94.35%	11.720%
15	8.854	2419	2430	2451	rBV	180932	300364	72.54%	9.012%
16	10.217	2844	2854	2868	rBV2	67504	107019	25.85%	3.211%
17	11.252	3165	3176	3195	rBV	170961	271158	65.49%	8.135%
18	11.535	3252	3264	3275	rBV3	5777	9759	2.36%	0.293%
19	11.625	3281	3292	3313	rBV	192324	301906	72.91%	9.058%
20	12.345	3508	3516	3529	rVB5	5656	8387	2.03%	0.252%




Sum of corrected areas: 3333118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022704.D
Acq On : 08 Oct 2021 15:44
Operator : SY/MD
Sample : M4098-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

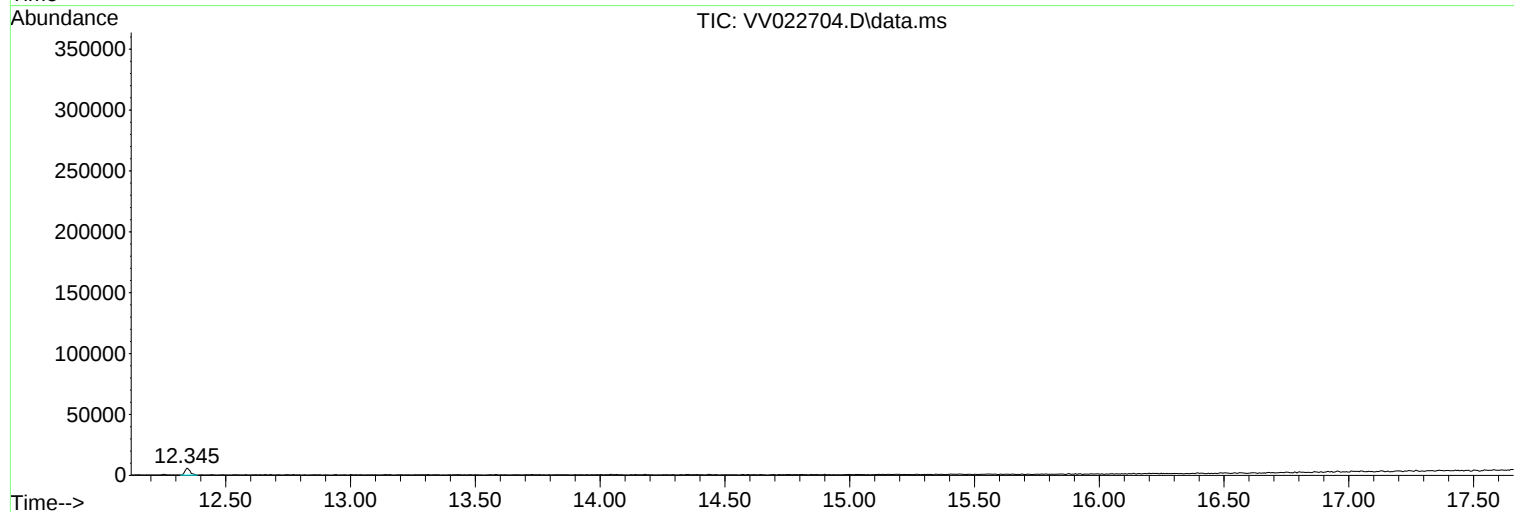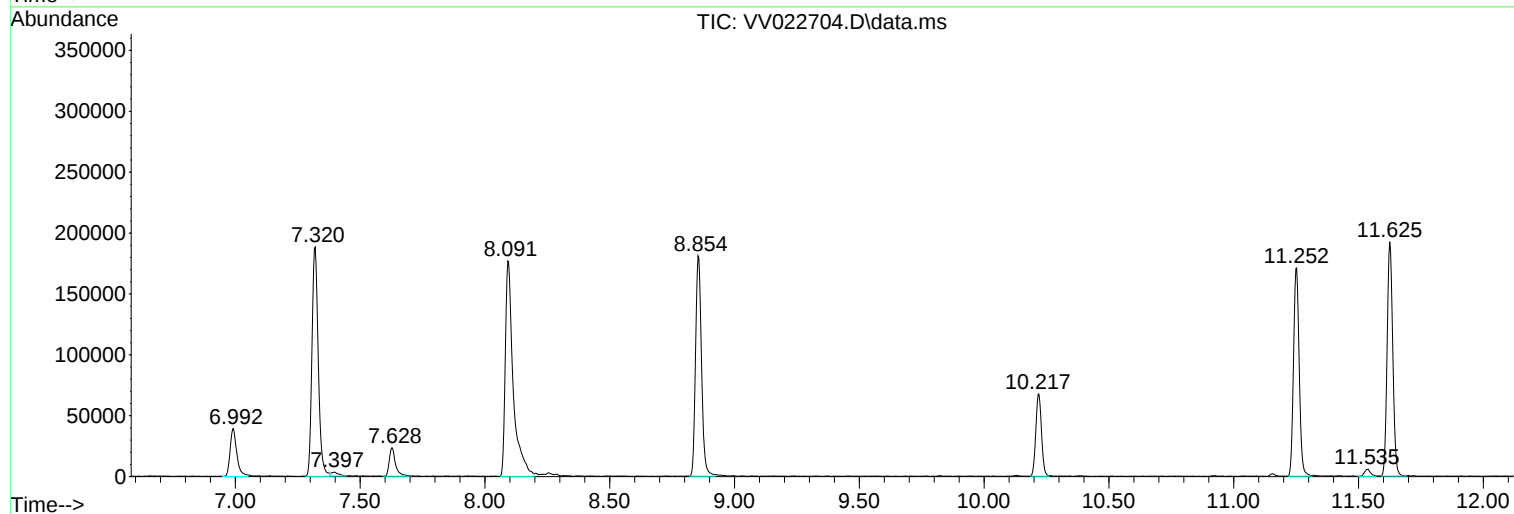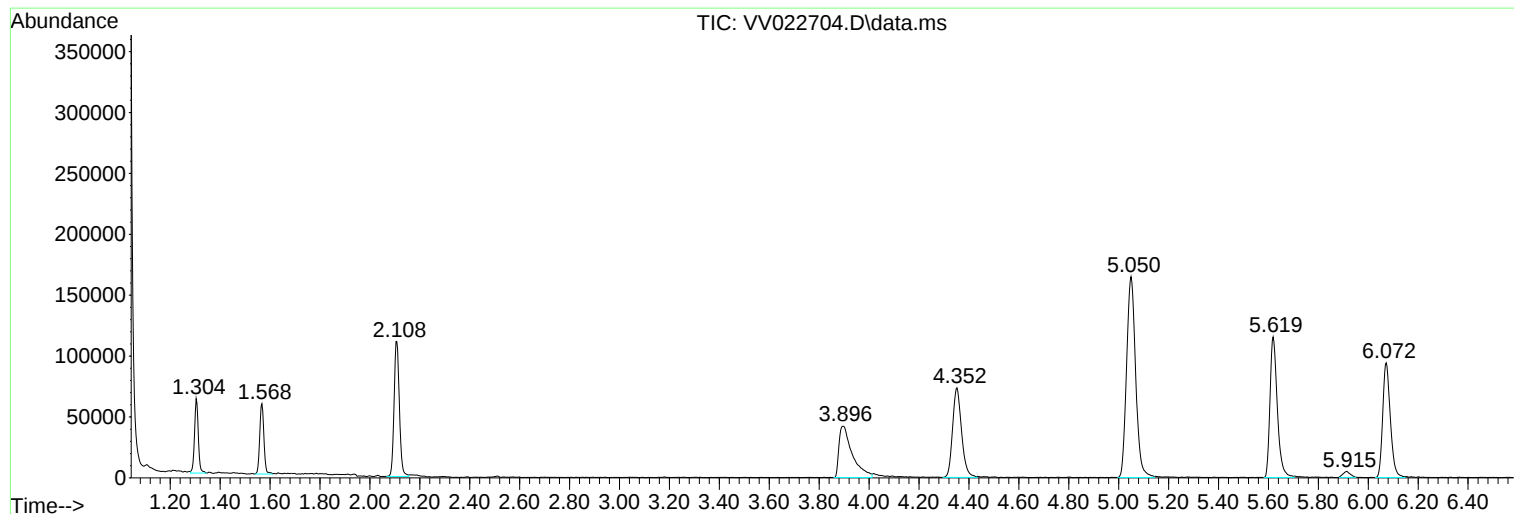

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022704.D
Acq On : 08 Oct 2021 15:44
Operator : SY/MD
Sample : M4098-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022704.D
Acq On : 08 Oct 2021 15:44
Operator : SY/MD
Sample : M4098-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
