

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022706.D
 Acq On : 08 Oct 2021 16:32
 Operator : SY/MD
 Sample : M4098-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT45

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	57541	57783	14.78%	1.811%
2	1.564	156	163	174	rBV	56561	64721	16.55%	2.028%
3	2.105	321	331	344	rBV	104333	152976	39.12%	4.794%
4	3.902	876	890	919	rBV	35543	135042	34.53%	4.232%
5	4.349	1013	1029	1052	rBV2	67549	174733	44.68%	5.476%
6	5.050	1231	1247	1277	rBV2	156296	391062	100.00%	12.255%
7	5.619	1412	1424	1446	rBV2	113583	234613	59.99%	7.352%
8	5.911	1503	1515	1528	rBV8	5149	11086	2.83%	0.347%
9	6.072	1552	1565	1583	rBV2	89649	184671	47.22%	5.787%
10	6.989	1840	1850	1865	rBV	36103	66831	17.09%	2.094%
11	7.320	1941	1953	1969	rBV	174841	308401	78.86%	9.665%
12	7.628	2039	2049	2065	rBV	21884	39687	10.15%	1.244%
13	7.943	2135	2147	2157	rBV2	11479	19893	5.09%	0.623%
14	8.095	2182	2194	2224	rBV2	173024	369209	94.41%	11.570%
15	8.853	2420	2430	2449	rBV	180710	299952	76.70%	9.400%
16	10.220	2843	2855	2870	rBV	63372	100868	25.79%	3.161%
17	10.384	2895	2906	2917	rVB2	14690	23974	6.13%	0.751%
18	11.252	3165	3176	3192	rBV	174518	270248	69.11%	8.469%
19	11.625	3281	3292	3309	rBV	178654	276567	70.72%	8.667%
20	12.249	3474	3486	3498	rVB	5606	8675	2.22%	0.272%




Sum of corrected areas: 3190992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022706.D
Acq On : 08 Oct 2021 16:32
Operator : SY/MD
Sample : M4098-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

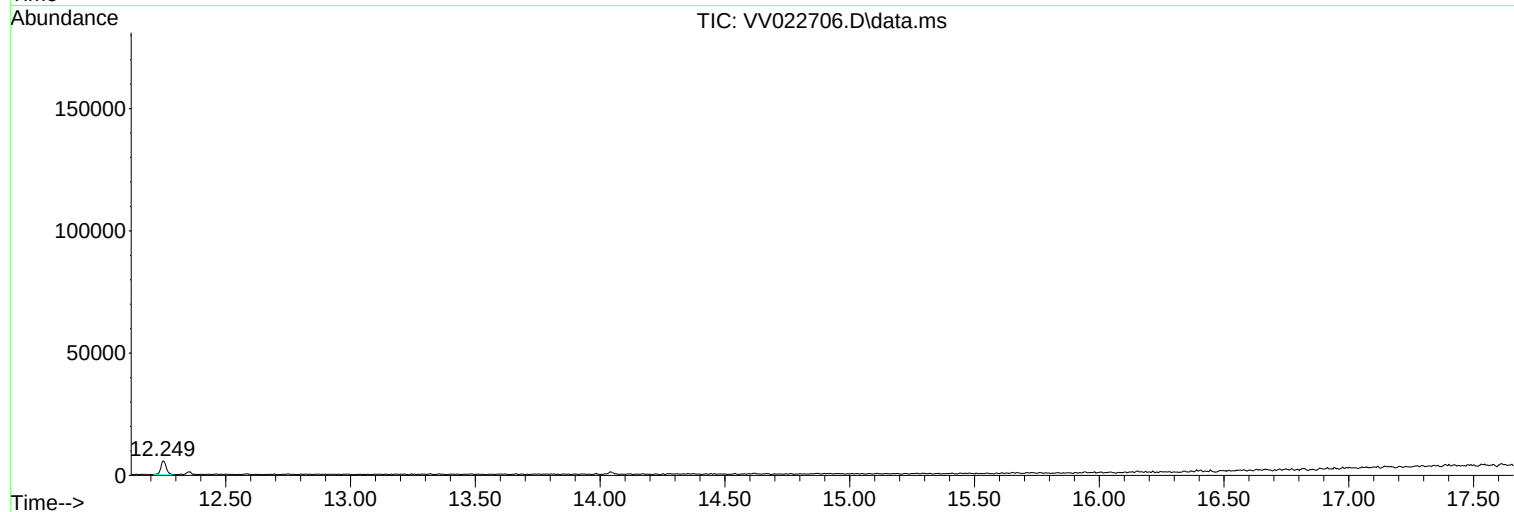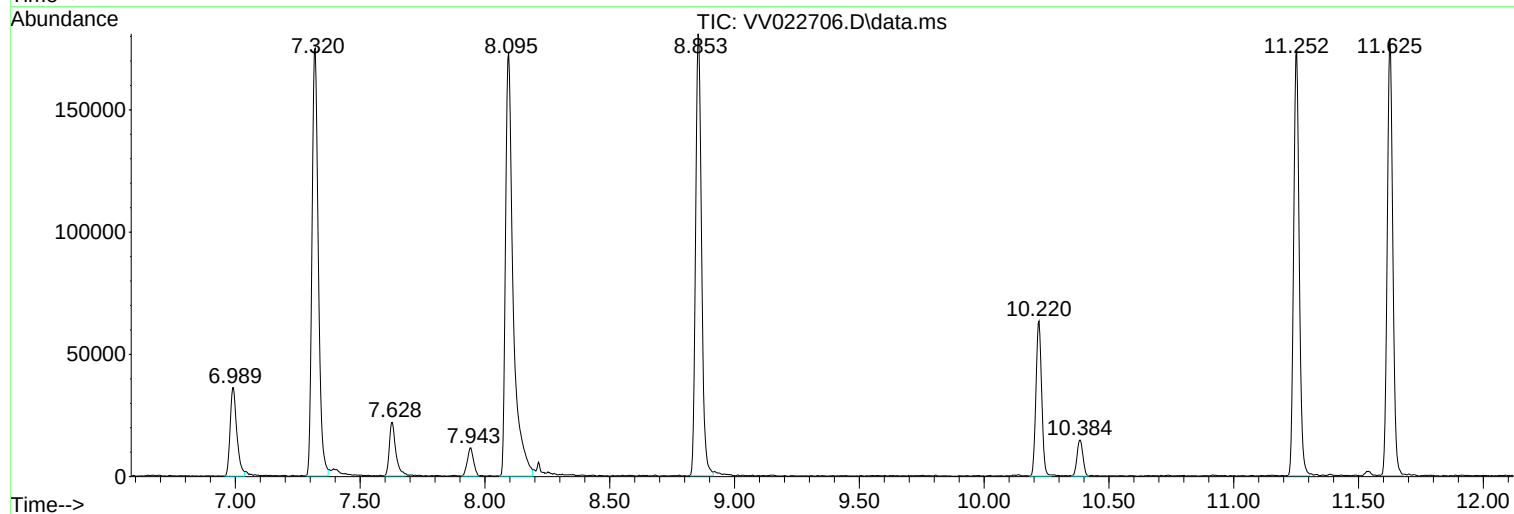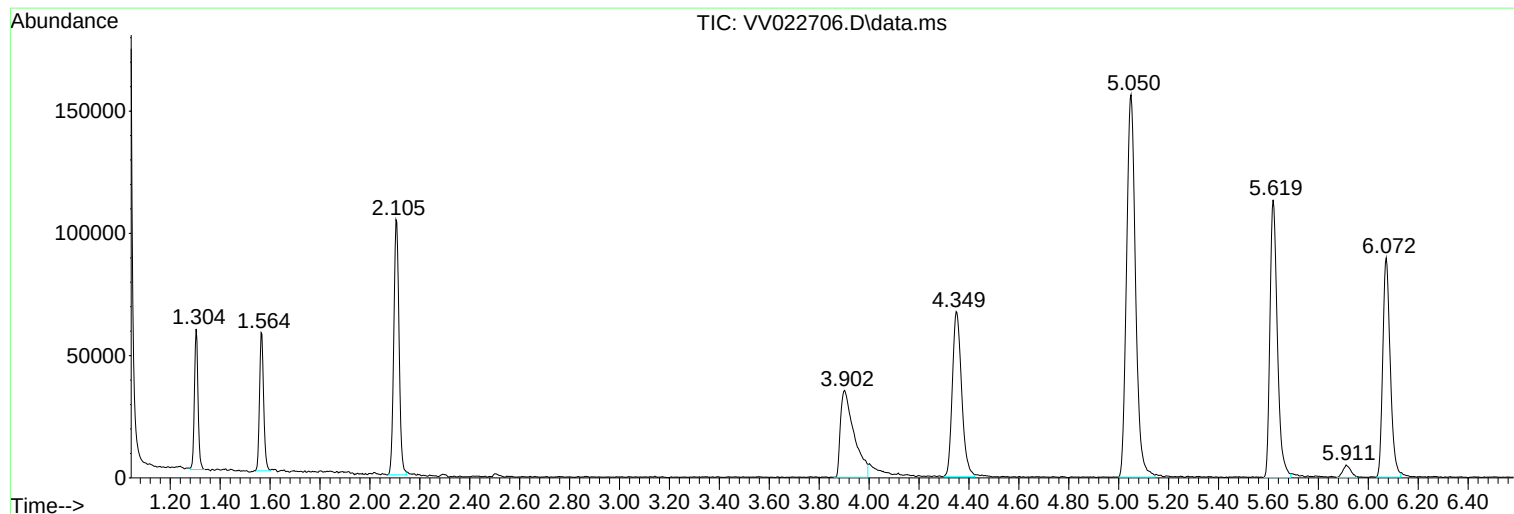

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022706.D
Acq On : 08 Oct 2021 16:32
Operator : SY/MD
Sample : M4098-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022706.D
Acq On : 08 Oct 2021 16:32
Operator : SY/MD
Sample : M4098-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
