

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022708.D
 Acq On : 08 Oct 2021 17:20
 Operator : SY/MD
 Sample : M4098-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAT33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	92	rVB	53486	55637	14.58%	1.788%
2	1.565	155	163	175	rBV	55737	62670	16.43%	2.014%
3	2.101	320	330	346	rBV	96601	139504	36.56%	4.482%
4	3.918	884	895	931	rBV2	28460	115859	30.37%	3.722%
5	4.346	1013	1028	1055	rVB	69348	173585	45.50%	5.577%
6	5.043	1230	1245	1267	rBV2	158085	381539	100.00%	12.259%
7	5.616	1410	1423	1449	rBV	117315	239985	62.90%	7.711%
8	5.905	1504	1513	1531	rBV6	4840	9385	2.46%	0.302%
9	6.072	1552	1565	1584	rBV	90928	183154	48.00%	5.885%
10	6.989	1838	1850	1867	rBV2	34316	65151	17.08%	2.093%
11	7.317	1941	1952	1970	rBV	167847	291413	76.38%	9.363%
12	7.625	2039	2048	2068	rBV2	20458	38926	10.20%	1.251%
13	7.944	2133	2147	2158	rBV2	7382	12729	3.34%	0.409%
14	8.098	2184	2195	2229	rBV3	142215	380581	99.75%	12.228%
15	8.854	2419	2430	2456	rBV	180198	300741	78.82%	9.663%
16	10.220	2844	2855	2869	rBV	63155	101596	26.63%	3.264%
17	10.384	2896	2906	2917	rVB3	11985	18151	4.76%	0.583%
18	11.252	3162	3176	3196	rBV	167545	265337	69.54%	8.525%
19	11.625	3280	3292	3312	rBV	172888	270013	70.77%	8.675%
20	12.252	3478	3487	3497	rBV2	4146	6486	1.70%	0.208%




Sum of corrected areas: 3112442

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022708.D
Acq On : 08 Oct 2021 17:20
Operator : SY/MD
Sample : M4098-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

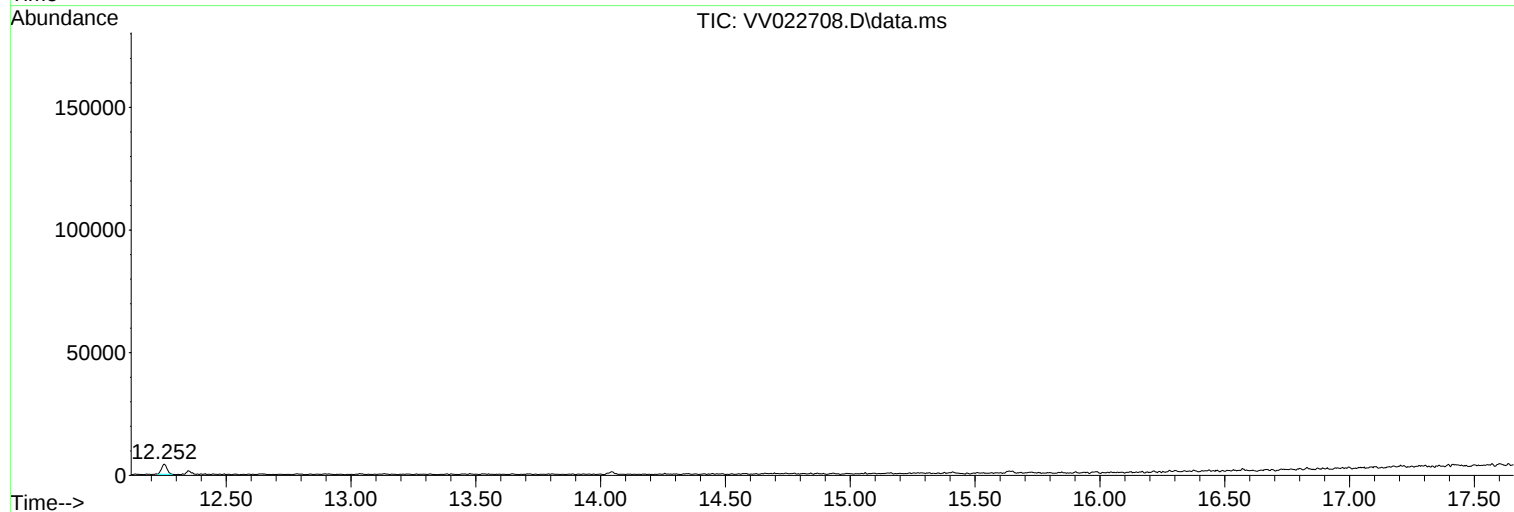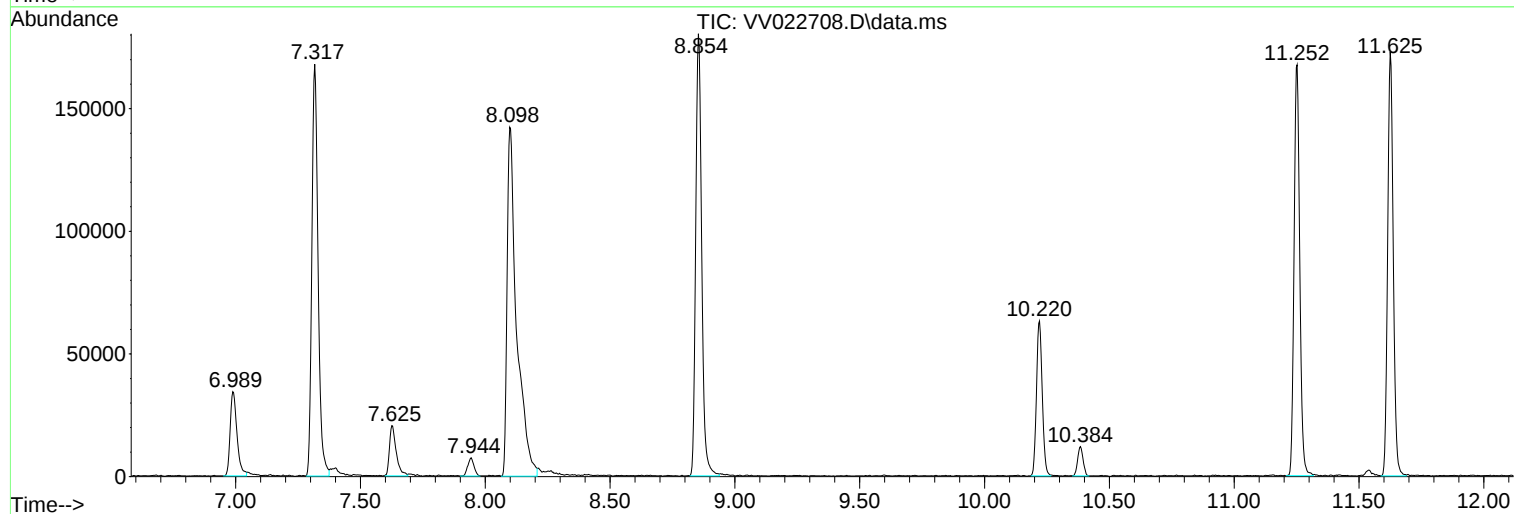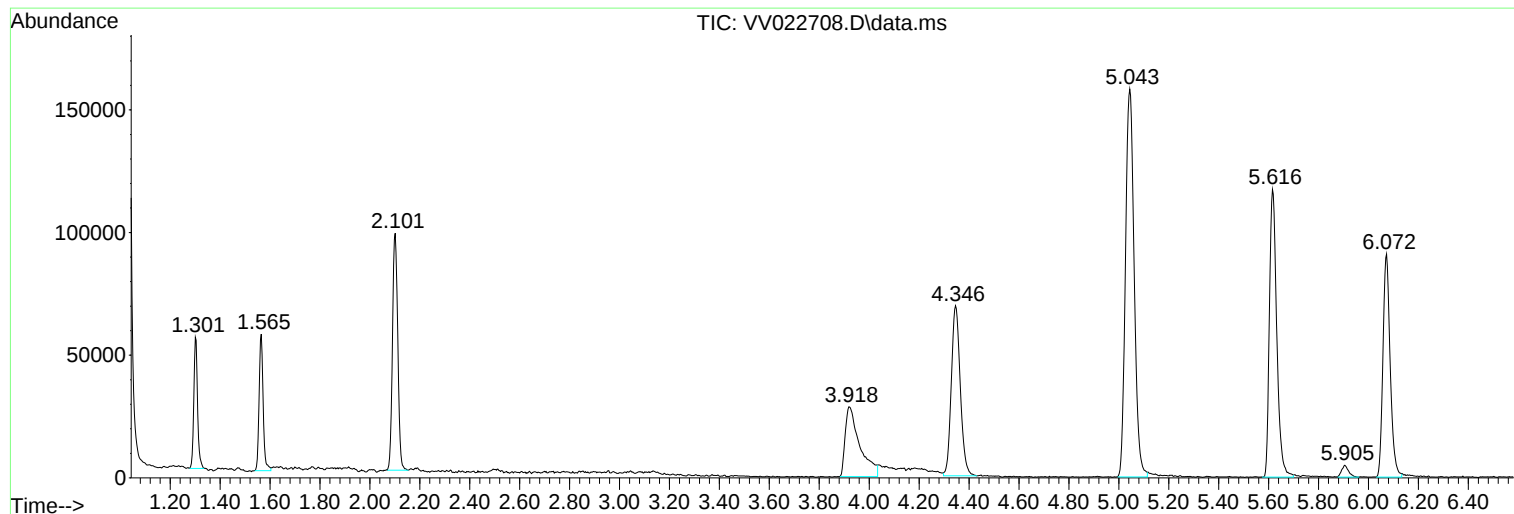

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022708.D
Acq On : 08 Oct 2021 17:20
Operator : SY/MD
Sample : M4098-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022708.D
Acq On : 08 Oct 2021 17:20
Operator : SY/MD
Sample : M4098-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAT33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
