

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022710.D
 Acq On : 08 Oct 2021 18:31
 Operator : SY/MD
 Sample : M4022-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0A27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	91	rBV	59353	59103	2.43%	0.900%
2	1.565	156	163	177	rBV	57479	65617	2.70%	0.999%
3	1.706	200	207	212	rBV	24568	28262	1.16%	0.430%
4	1.751	212	221	239	rVB	215686	283769	11.67%	4.321%
5	2.105	319	331	350	rBV	107519	156702	6.45%	2.386%
6	3.918	878	895	915	rBV4	35801	137028	5.64%	2.087%
7	4.346	1010	1028	1052	rVB	77877	200547	8.25%	3.054%
8	5.043	1229	1245	1277	rBV3	185999	430044	17.69%	6.549%
9	5.616	1410	1423	1447	rBV	131344	268176	11.03%	4.084%
10	5.912	1501	1515	1540	rBV	204317	401790	16.53%	6.119%
11	6.072	1550	1565	1586	rBV	98964	200249	8.24%	3.050%
12	6.989	1837	1850	1868	rBV2	39026	73861	3.04%	1.125%
13	7.317	1936	1952	1972	rBV	193907	340904	14.02%	5.192%
14	7.625	2039	2048	2066	rBV	24386	43272	1.78%	0.659%
15	7.976	2137	2157	2185	rBV	1449897	2430854	100.00%	37.019%
16	8.101	2185	2196	2241	rVB2	160735	420622	17.30%	6.406%
17	8.854	2419	2430	2452	rBV	194125	331312	13.63%	5.045%
18	10.220	2842	2855	2870	rBV	65401	106154	4.37%	1.617%
19	11.249	3164	3175	3195	rBV	185325	291869	12.01%	4.445%
20	11.625	3281	3292	3315	rBV	187919	296386	12.19%	4.514%




Sum of corrected areas: 6566521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022710.D
Acq On : 08 Oct 2021 18:31
Operator : SY/MD
Sample : M4022-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

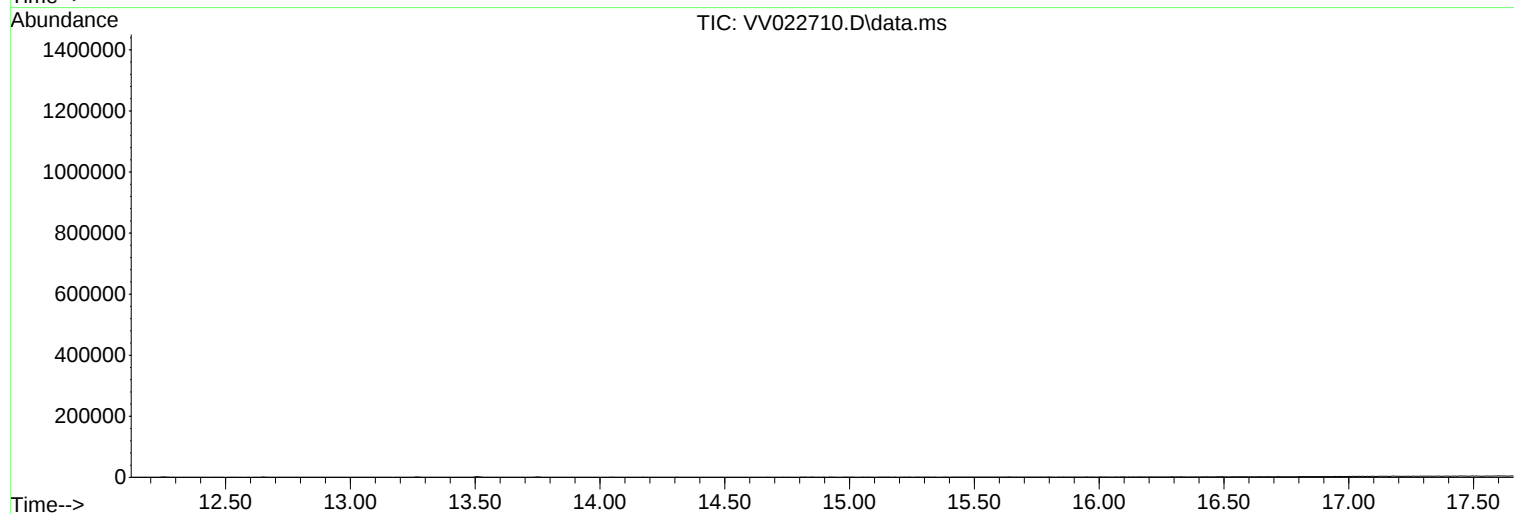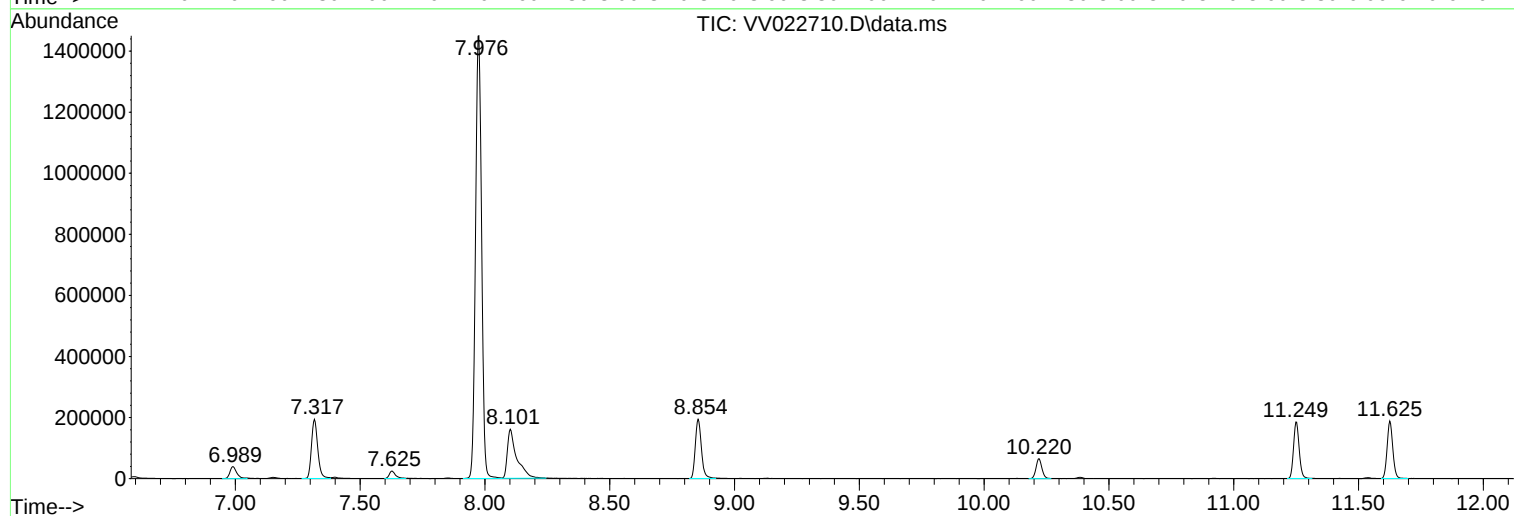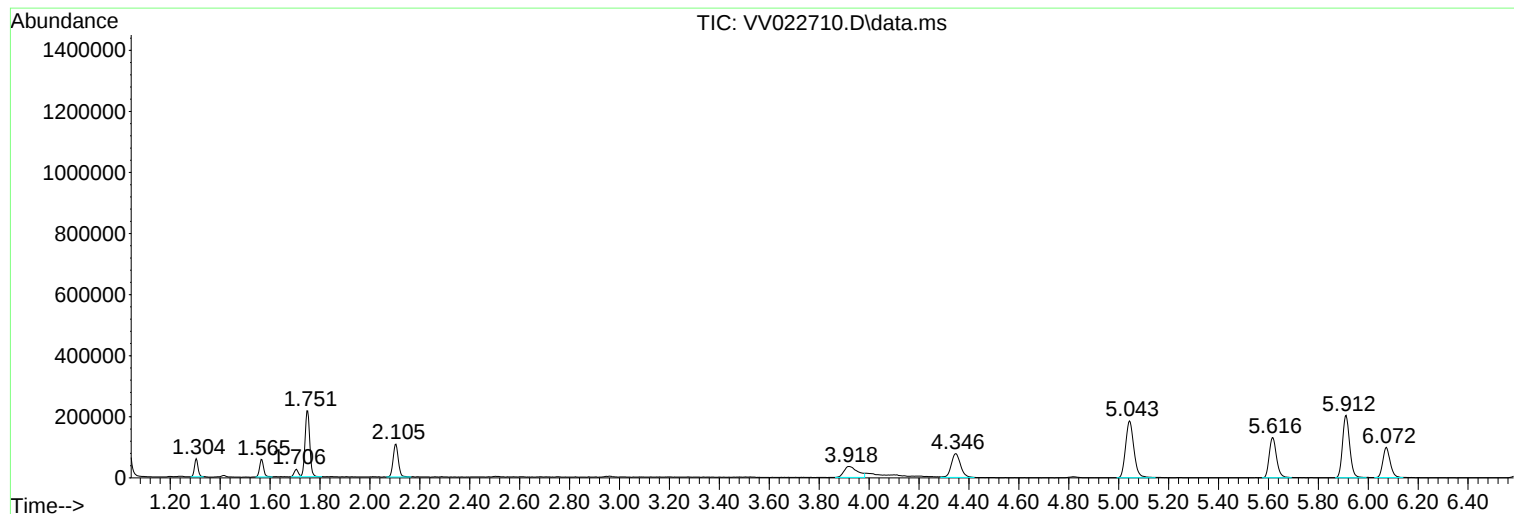

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022710.D
Acq On : 08 Oct 2021 18:31
Operator : SY/MD
Sample : M4022-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022710.D
Acq On : 08 Oct 2021 18:31
Operator : SY/MD
Sample : M4022-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
