

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022711.D
 Acq On : 08 Oct 2021 18:55
 Operator : SY/MD
 Sample : M4022-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	57892	58367	1.79%	0.806%
2	1.565	156	163	174	rBV	56180	64913	2.00%	0.897%
3	1.751	212	221	238	rVB	362700	473411	14.56%	6.540%
4	2.105	321	331	342	rBV	106997	153092	4.71%	2.115%
5	3.915	880	894	922	rBV2	36101	134134	4.12%	1.853%
6	4.346	1012	1028	1050	rVB	77088	197495	6.07%	2.728%
7	5.043	1228	1245	1267	rBV2	181985	424094	13.04%	5.859%
8	5.616	1411	1423	1445	rBV	129064	255820	7.87%	3.534%
9	5.912	1501	1515	1536	rBV2	68431	140861	4.33%	1.946%
10	6.072	1550	1565	1585	rBV	99193	203093	6.25%	2.806%
11	6.989	1840	1850	1866	rBV	40242	72955	2.24%	1.008%
12	7.317	1938	1952	1971	rBV	193706	339992	10.46%	4.697%
13	7.625	2039	2048	2063	rBV	22836	42403	1.30%	0.586%
14	7.976	2135	2157	2185	rBV	1957114	3251897	100.00%	44.925%
15	8.098	2185	2195	2232	rVB2	159634	407524	12.53%	5.630%
16	8.854	2416	2430	2452	rBV	196162	331145	10.18%	4.575%
17	10.220	2844	2855	2872	rBV2	65745	106597	3.28%	1.473%
18	11.249	3165	3175	3199	rBV	182883	287541	8.84%	3.972%
19	11.625	3279	3292	3309	rBV	184130	293161	9.02%	4.050%




Sum of corrected areas: 7238495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022711.D
Acq On : 08 Oct 2021 18:55
Operator : SY/MD
Sample : M4022-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

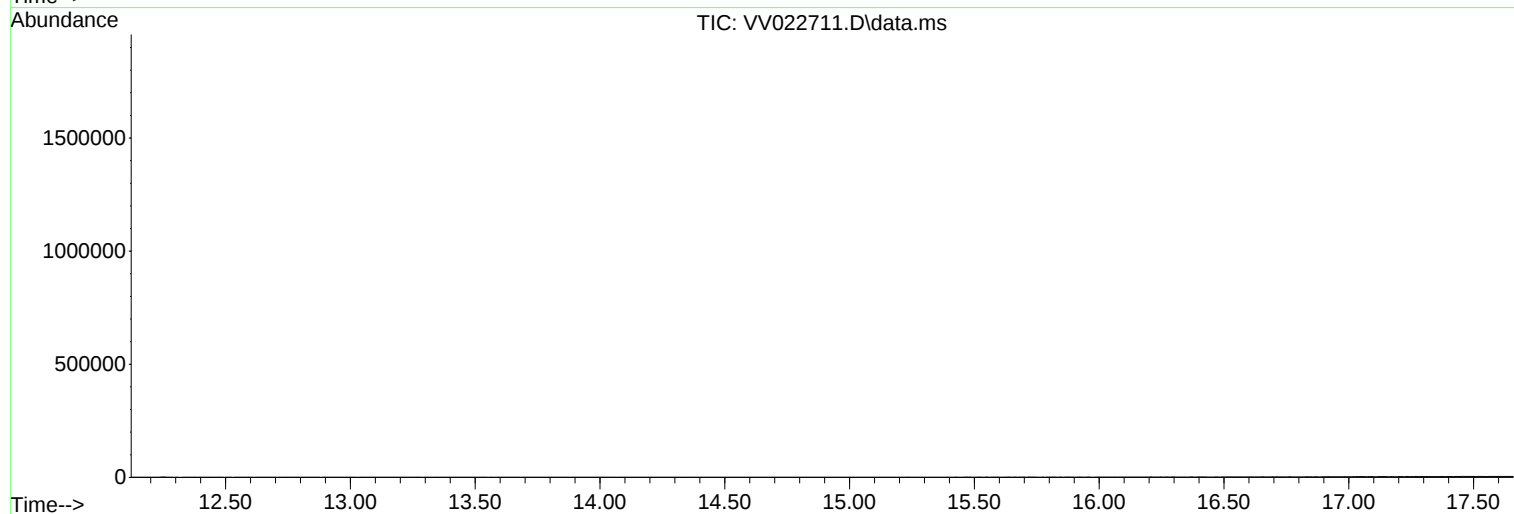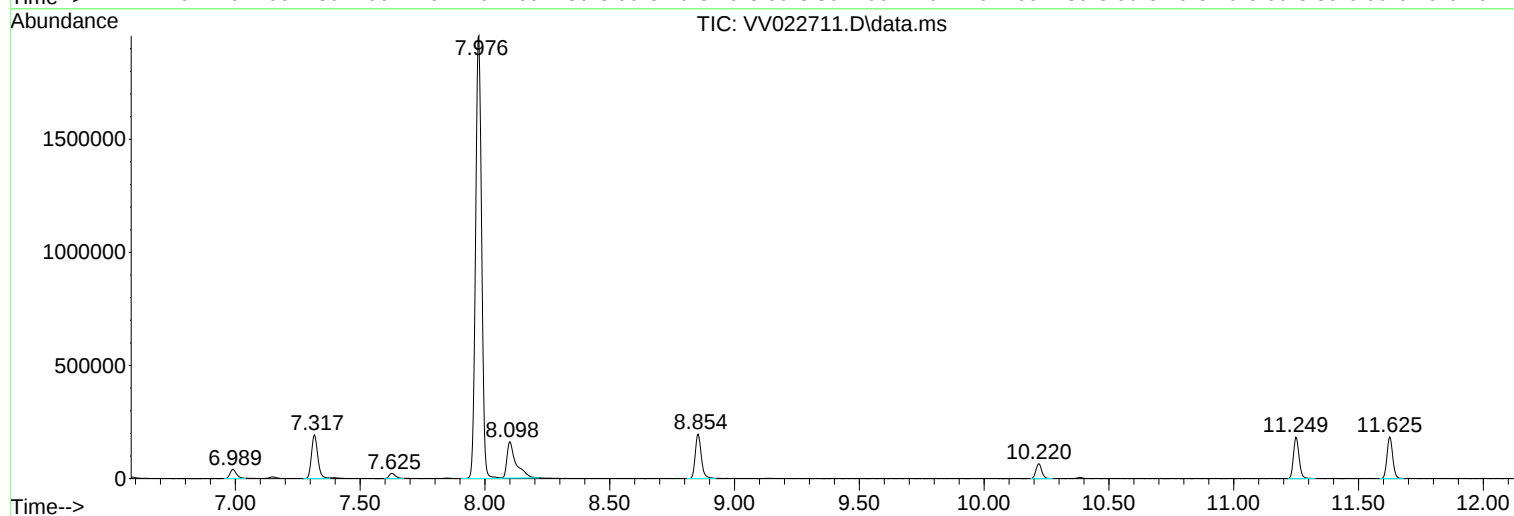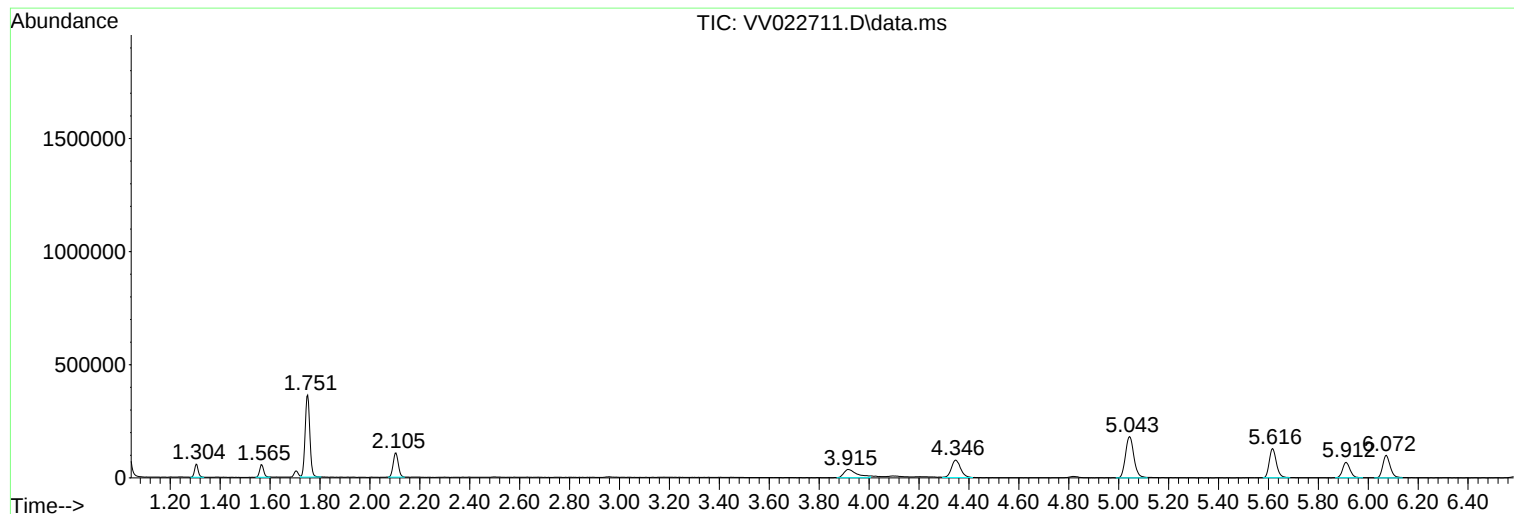

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022711.D
Acq On : 08 Oct 2021 18:55
Operator : SY/MD
Sample : M4022-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022711.D
Acq On : 08 Oct 2021 18:55
Operator : SY/MD
Sample : M4022-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
