

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
 Data File : VV022712.D
 Acq On : 08 Oct 2021 19:19
 Operator : SY/MD
 Sample : M4022-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	57886	58153	4.42%	1.040%
2	1.568	156	164	174	rBV	55008	62884	4.78%	1.125%
3	1.706	198	207	212	rBV	32442	39633	3.01%	0.709%
4	1.748	212	220	236	rVB	295437	386984	29.40%	6.922%
5	2.101	320	330	344	rBV	104464	149021	11.32%	2.665%
6	3.918	879	895	931	rBV4	40591	162504	12.35%	2.907%
7	4.346	1013	1028	1052	rVB	75940	191388	14.54%	3.423%
8	5.043	1229	1245	1274	rBV3	179255	414630	31.50%	7.416%
9	5.616	1411	1423	1444	rBV	123627	252387	19.18%	4.514%
10	5.912	1500	1515	1536	rBV	250703	494434	37.56%	8.844%
11	6.072	1552	1565	1586	rBV	95251	196341	14.92%	3.512%
12	6.590	1713	1726	1741	rBV4	7237	16746	1.27%	0.300%
13	6.989	1840	1850	1867	rBV	39057	72395	5.50%	1.295%
14	7.149	1890	1900	1913	rBV5	7789	14959	1.14%	0.268%
15	7.317	1939	1952	1970	rBV	187440	328977	24.99%	5.884%
16	7.625	2039	2048	2065	rBV	23112	40647	3.09%	0.727%
17	7.976	2137	2157	2185	rBV	794759	1316215	100.00%	23.542%
18	8.098	2185	2195	2237	rVV3	153012	400259	30.41%	7.159%
19	8.854	2419	2430	2453	rBV	194800	321360	24.42%	5.748%
20	10.220	2840	2855	2871	rBV	64471	103652	7.88%	1.854%
21	11.249	3165	3175	3191	rBV	182095	281286	21.37%	5.031%
22	11.625	3279	3292	3312	rBV	182734	285949	21.73%	5.115%




Sum of corrected areas: 5590804

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022712.D
Acq On : 08 Oct 2021 19:19
Operator : SY/MD
Sample : M4022-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

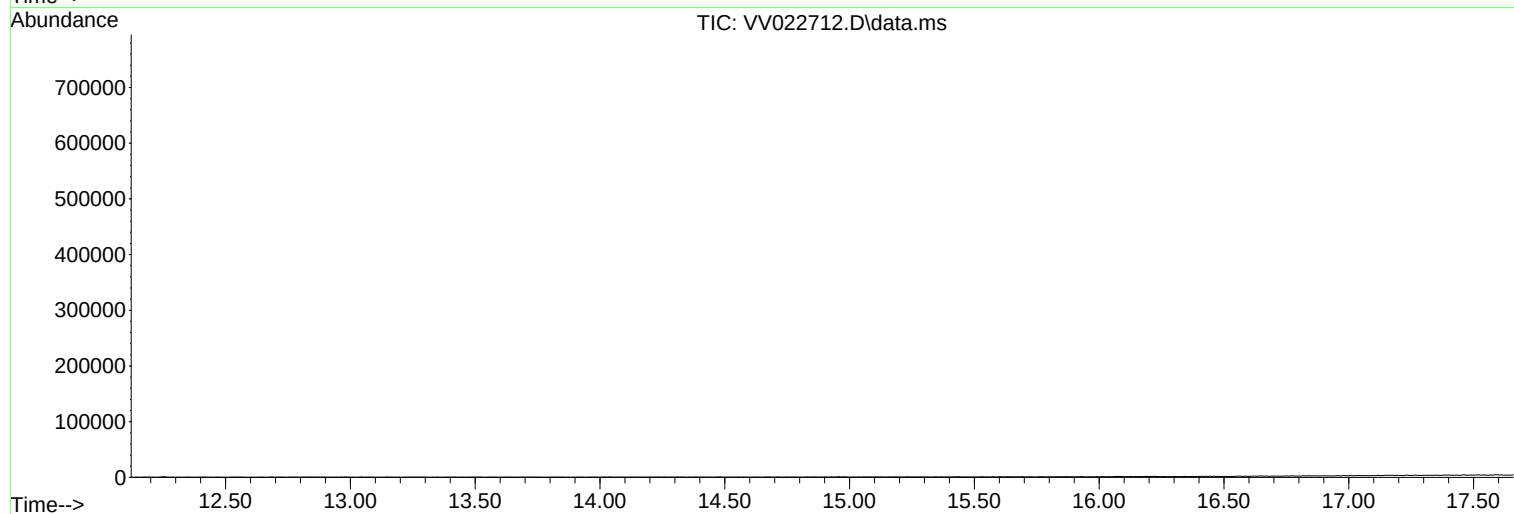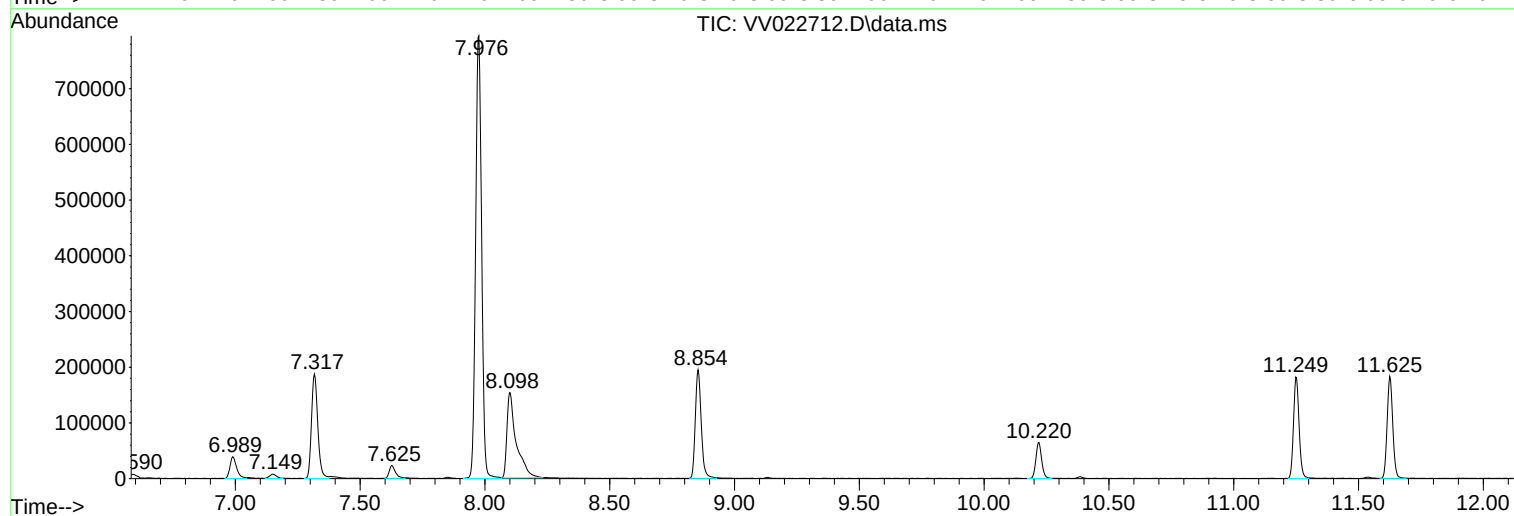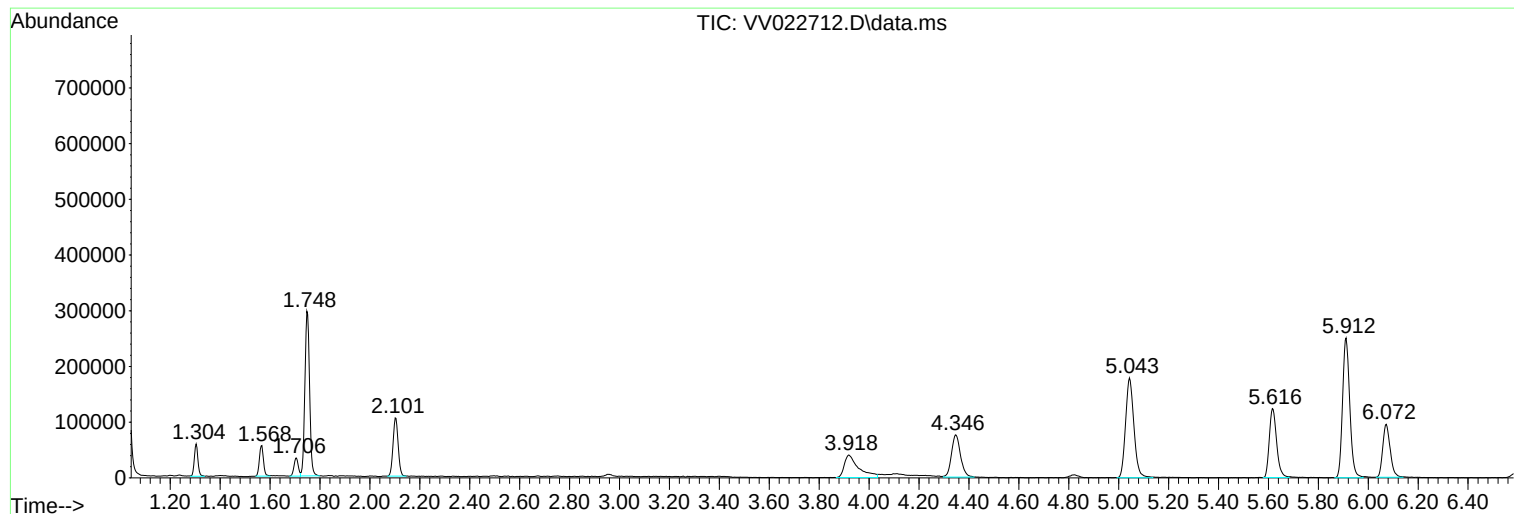

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022712.D
Acq On : 08 Oct 2021 19:19
Operator : SY/MD
Sample : M4022-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100821\
Data File : VV022712.D
Acq On : 08 Oct 2021 19:19
Operator : SY/MD
Sample : M4022-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
