

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
 Data File : VV008201.D
 Acq On : 09 Oct 2018 14:58
 Operator : SY/MD
 Sample : J5281-17
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYM4

Quant Time: Oct 10 04:25:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 10 03:08:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89047	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85663	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	38385	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	25148	4.60	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.00%
7) Chloroethane-d5	1.59	69	21242	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.14	63	36793	3.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.80%
20) 2-Butanone-d5	3.97	46	69920	53.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.34%
24) Chloroform-d	4.41	84	54525	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
26) 1,2-Dichloroethane-d4	5.09	65	27604	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.10	84	104847	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.13	67	33981	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.36	98	93838	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
43) trans-1,3-Dichloropropene-	7.67	79	10978	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.14	63	40927	42.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22679	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	37890	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	2377	2.668 ug/L	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
Data File : VV008201.D
Acq On : 09 Oct 2018 14:58
Operator : SY/MD
Sample : J5281-17
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYM4

Quant Time: Oct 10 04:25:40 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 10 03:08:28 2018
Response via : Initial Calibration

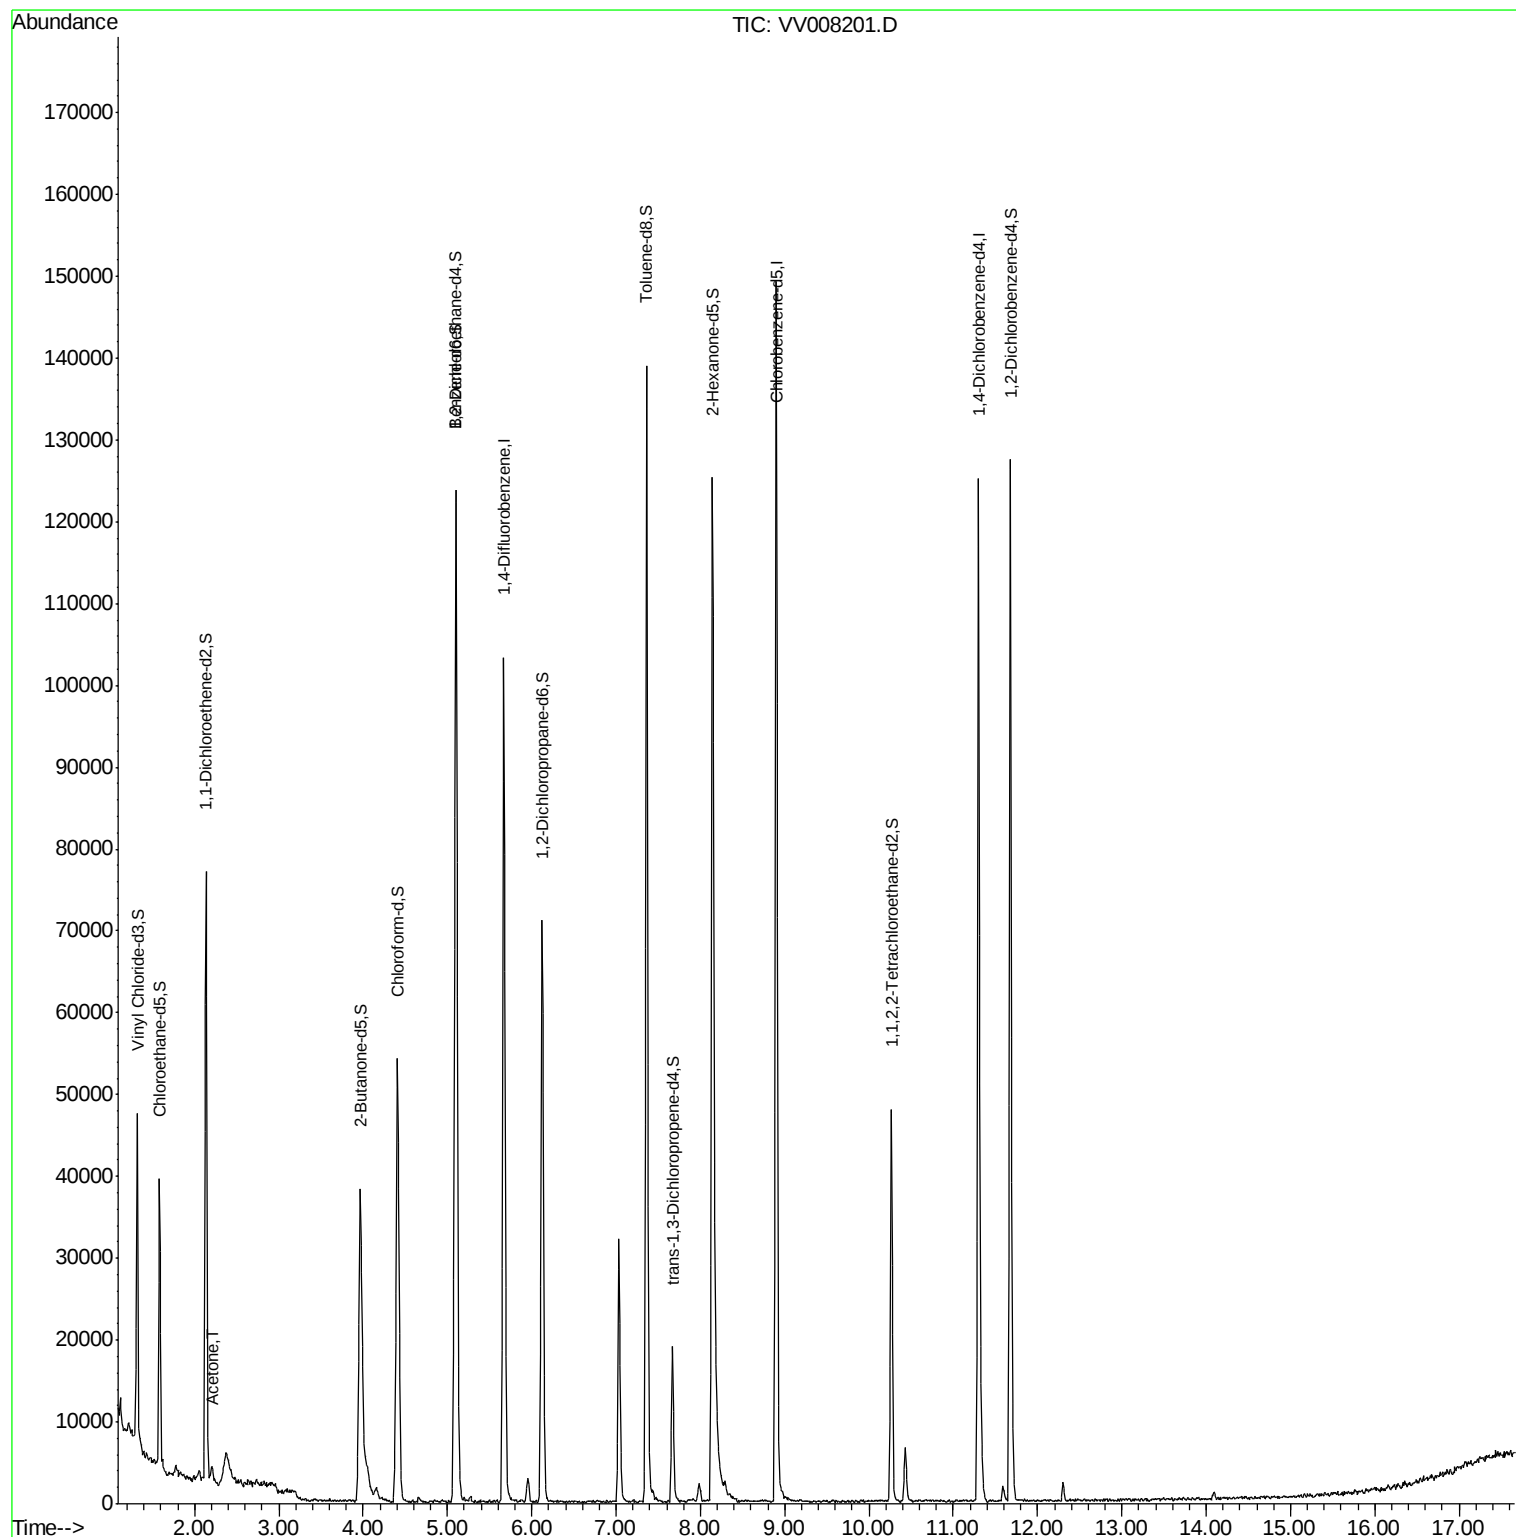

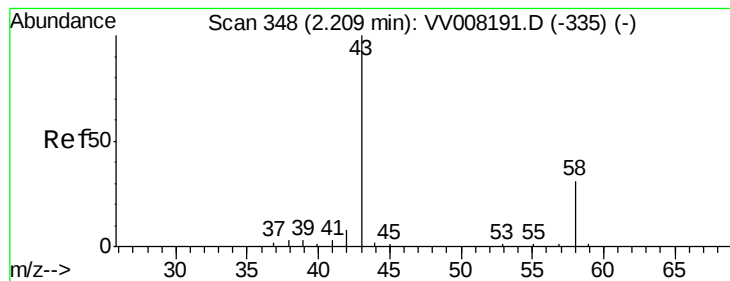

#13
 Acetone
 Concen: 2.668 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. 0.01 min
 Lab File: VV008201.D
 Acq: 09 Oct 2018 14:58

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYM4

Tot Ion: 43 Resp: 2377
 Ion Ratio Lower Upper
 43 100
 58 14.6 0.0 62.2

