

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
 Data File : VV008203.D
 Acq On : 09 Oct 2018 15:53
 Operator : SY/MD
 Sample : J5281-19
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYM6

Quant Time: Oct 10 04:32:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 10 03:08:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	88340	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	87209	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	39678	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24326	4.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.80%
7) Chloroethane-d5	1.59	69	21182	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.60%
11) 1,1-Dichloroethene-d2	2.14	63	37656	3.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.00%
20) 2-Butanone-d5	3.96	46	67612	51.83	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.66%
24) Chloroform-d	4.41	84	53725	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.09	65	27314	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.10	84	105139	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.13	67	33340	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.36	98	91663	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.67	79	10819	4.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.80%
46) 2-Hexanone-d5	8.14	63	41834	42.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.32%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22438	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	37500	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	1910	2.161 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100918\
Data File : VV008203.D
Acq On : 09 Oct 2018 15:53
Operator : SY/MD
Sample : J5281-19
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYM6

Quant Time: Oct 10 04:32:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 10 03:08:28 2018
Response via : Initial Calibration

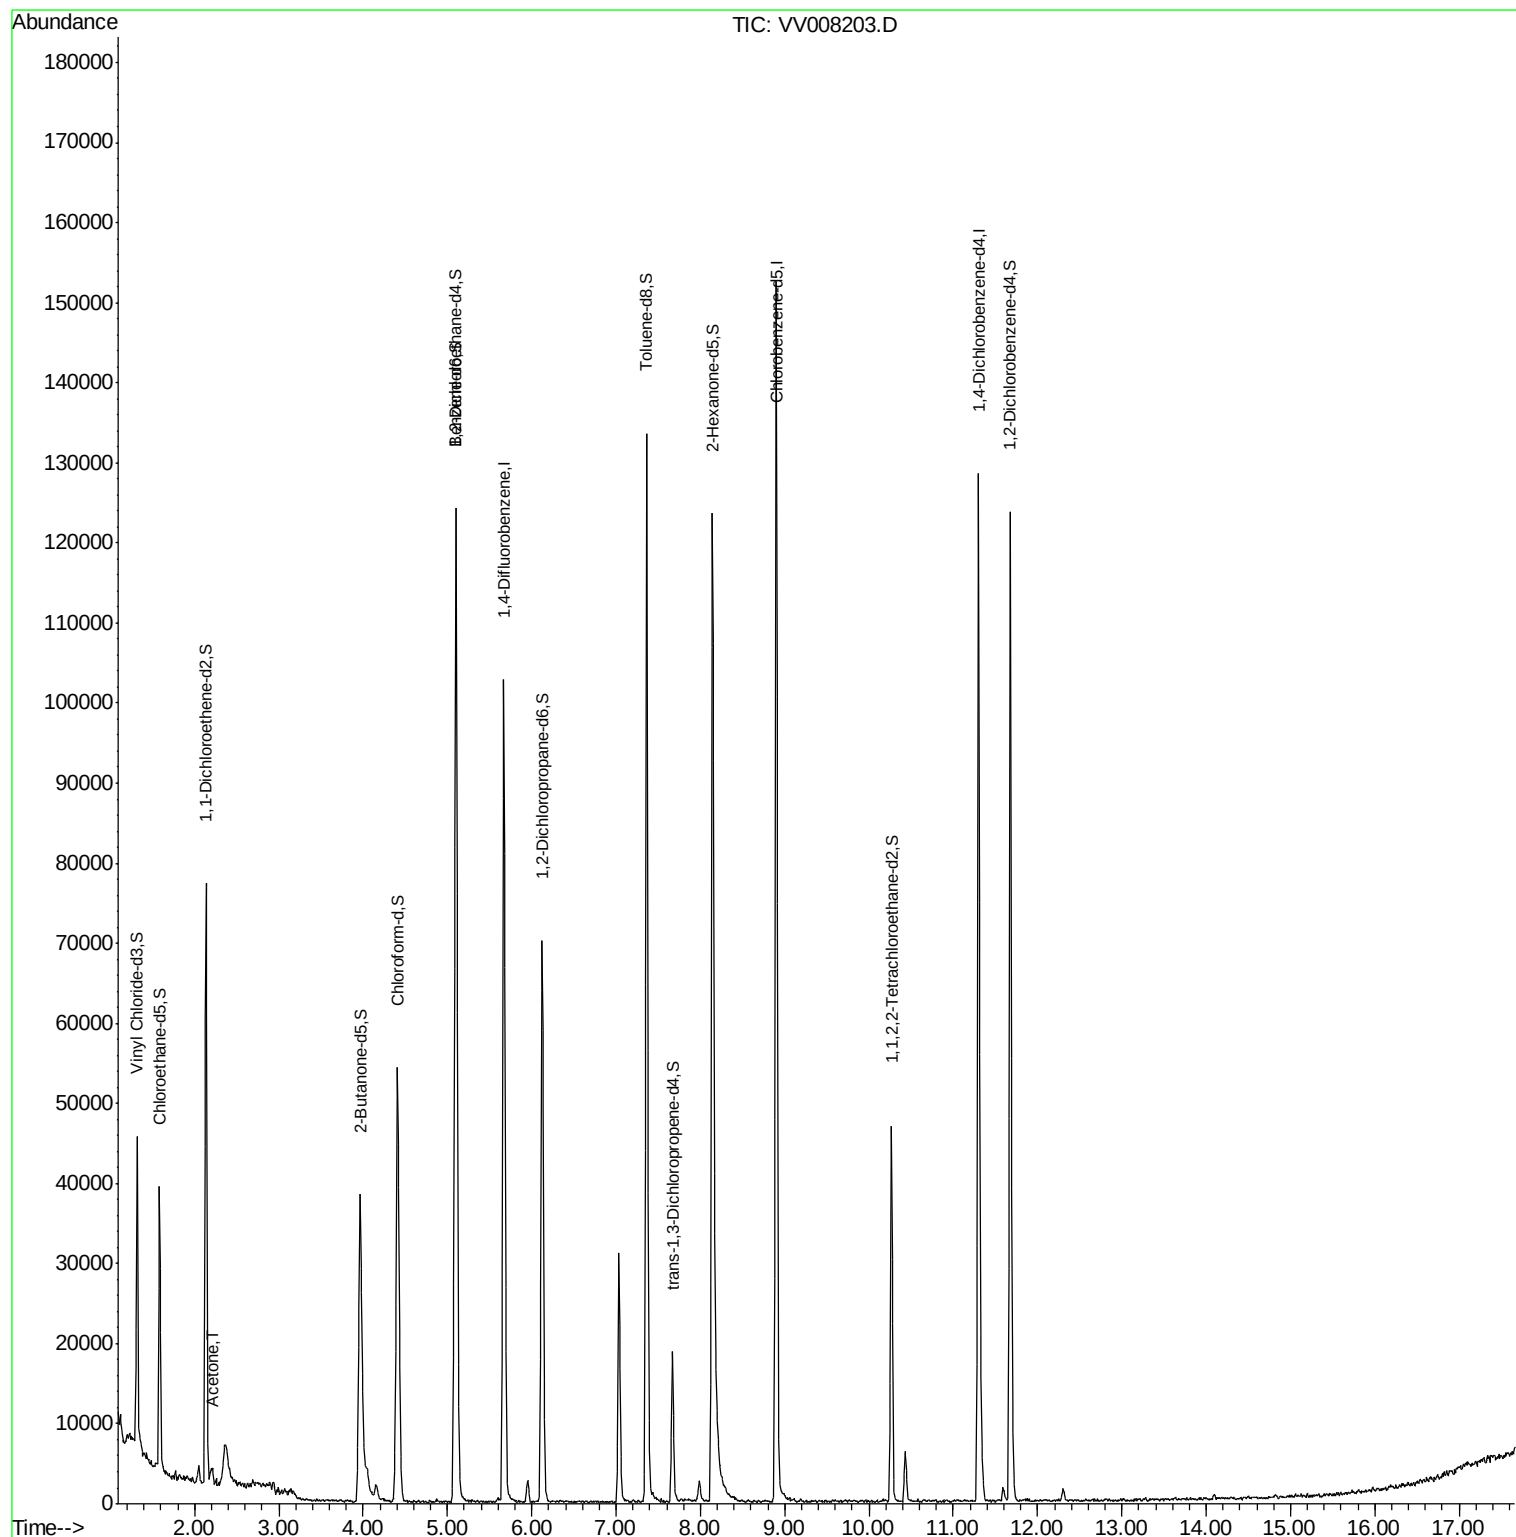

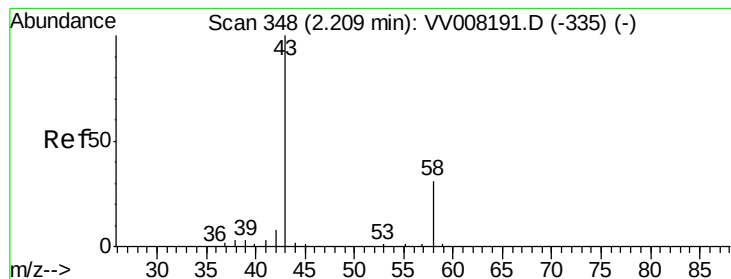

#13
 Acetone
 Concen: 2.161 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. 0.00 min
 Lab File: VV008203.D
 Acq: 09 Oct 2018 15:53

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYM6

Tot Ion: 43 Resp: 1910
 Ion Ratio Lower Upper
 43 100
 58 21.6 0.0 62.2

