

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
 Data File : VV008209.D
 Acq On : 09 Oct 2018 19:37
 Operator : SY/MD
 Sample : J5282-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYM8

Quant Time: Oct 10 04:46:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 10 03:08:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	89603	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	88948	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	39511	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	25683	4.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.40%
7) Chloroethane-d5	1.59	69	21893	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.40%
11) 1,1-Dichloroethene-d2	2.14	63	38113	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	3.96	46	82842	62.61	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.22%
24) Chloroform-d	4.41	84	57463	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.09	65	30343	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.10	84	109514	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
36) 1,2-Dichloropropane-d6	6.12	67	36296	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.36	98	95557	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
43) trans-1,3-Dichloropropene-	7.67	79	11893	4.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.80%
46) 2-Hexanone-d5	8.14	63	51713	51.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.40%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	26768	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	41679	5.56	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	2542	2.835 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100918\
Data File : VV008209.D
Acq On : 09 Oct 2018 19:37
Operator : SY/MD
Sample : J5282-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYM8

Quant Time: Oct 10 04:46:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 10 03:08:28 2018
Response via : Initial Calibration

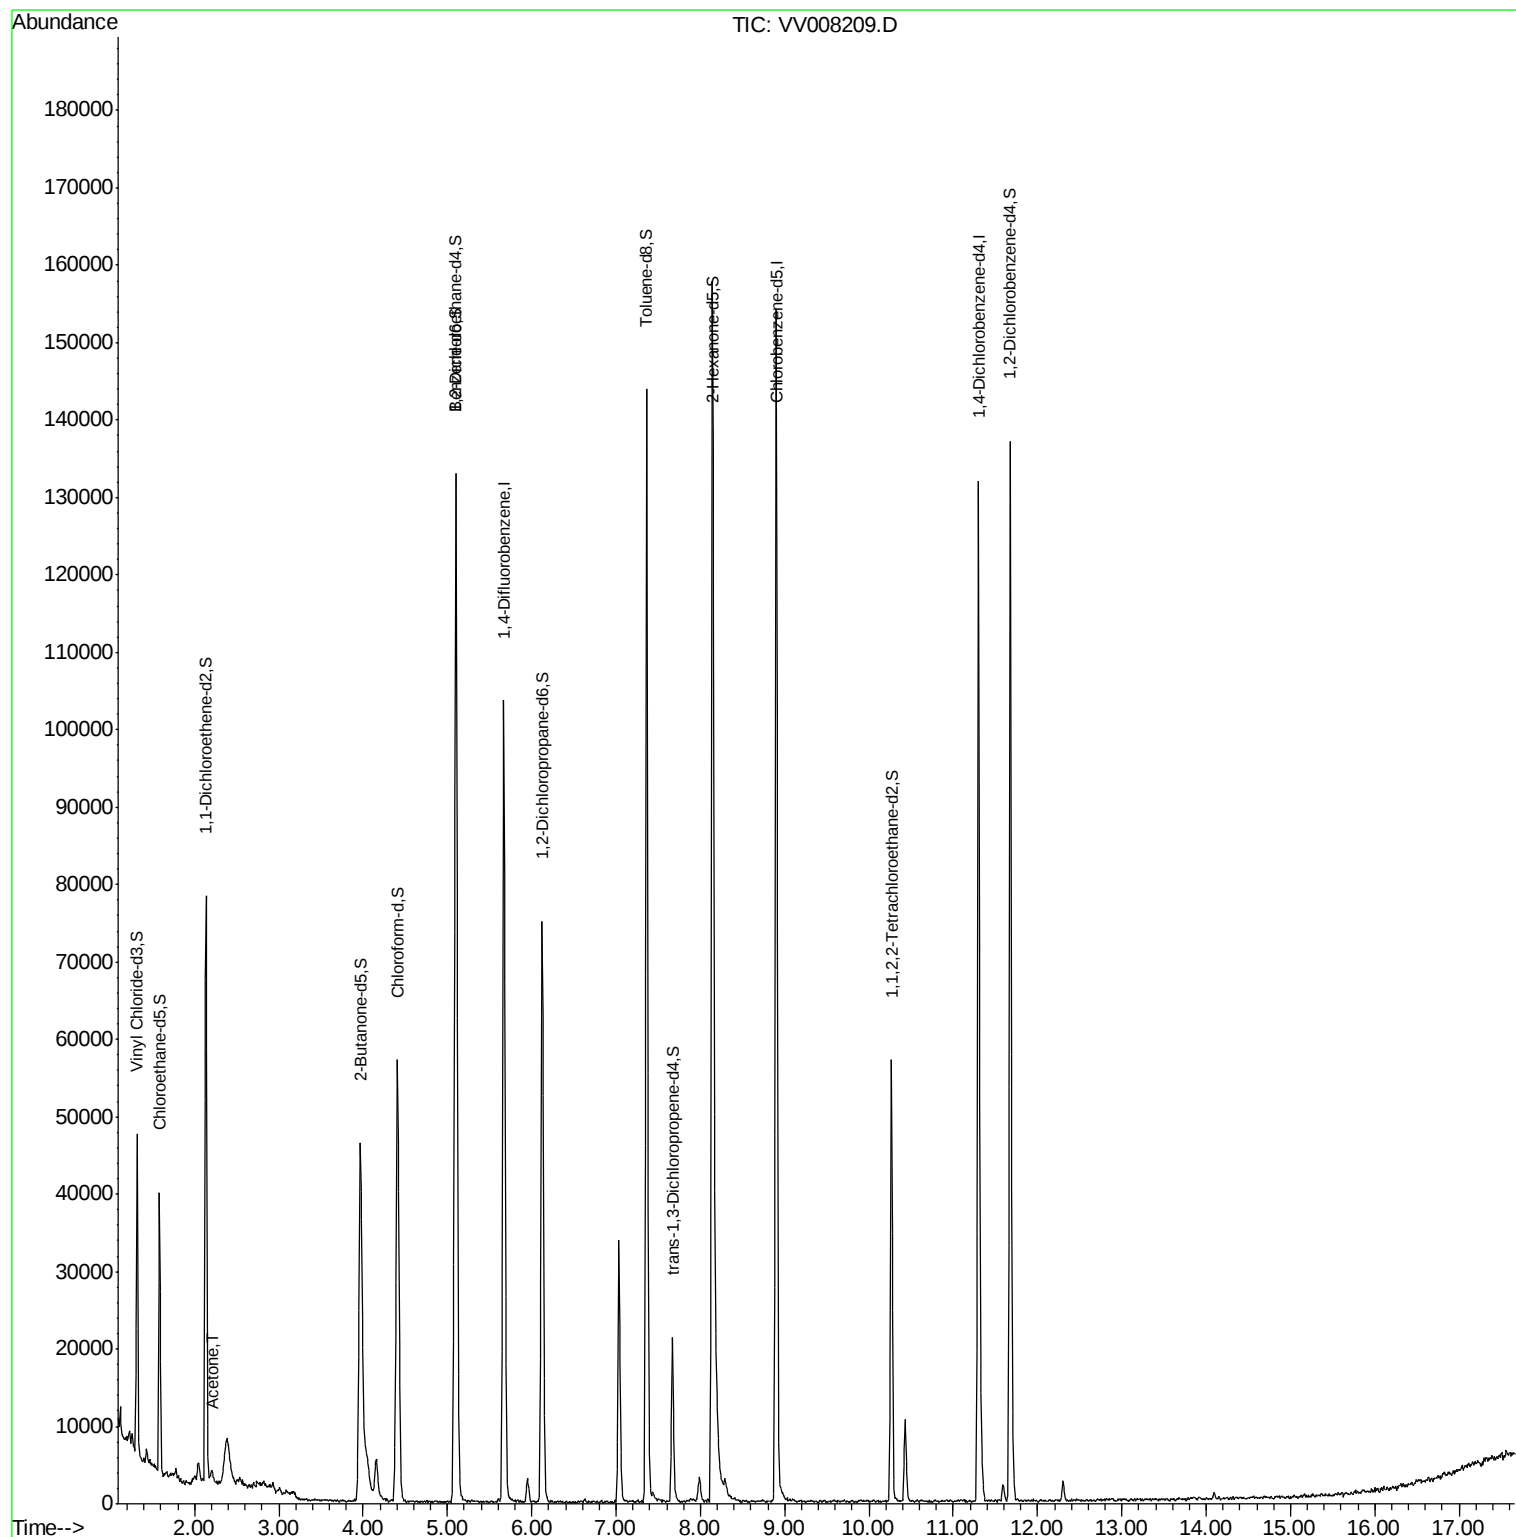

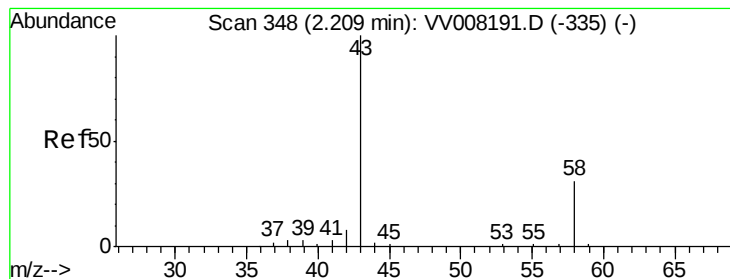

#13

Acetone

Concen: 2.835 ug/L

RT: 2.21 min Scan# 349

Delta R.T. 0.00 min

Lab File: VV008209.D

Acq: 09 Oct 2018 19:37

Instrument :
MSVOA_V
ClientSampleId :
BEYM8

Tot Ion: 43 Resp: 2542

Ion Ratio Lower Upper

43 100

58 24.9 0.0 62.2

