

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
 Data File : VV008214.D
 Acq On : 09 Oct 2018 22:21
 Operator : SY/MD
 Sample : J5282-04
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYN1

Quant Time: Oct 10 05:00:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 10 04:51:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	91542	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	90172	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41508	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23596	4.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.00%
7) Chloroethane-d5	1.59	69	20945	4.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.40%
11) 1,1-Dichloroethene-d2	2.14	63	35194	3.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.00%
20) 2-Butanone-d5	3.97	46	79397	58.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.46%
24) Chloroform-d	4.41	84	55712	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.09	65	28693	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.10	84	104437	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.13	67	34288	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.36	98	90538	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.80%
43) trans-1,3-Dichloropropene-	7.67	79	11203	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.14	63	51230	50.52	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.04%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24960	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	38194	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	2252	2.459 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100918\
Data File : VV008214.D
Acq On : 09 Oct 2018 22:21
Operator : SY/MD
Sample : J5282-04
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYN1

Quant Time: Oct 10 05:00:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 10 04:51:19 2018
Response via : Initial Calibration

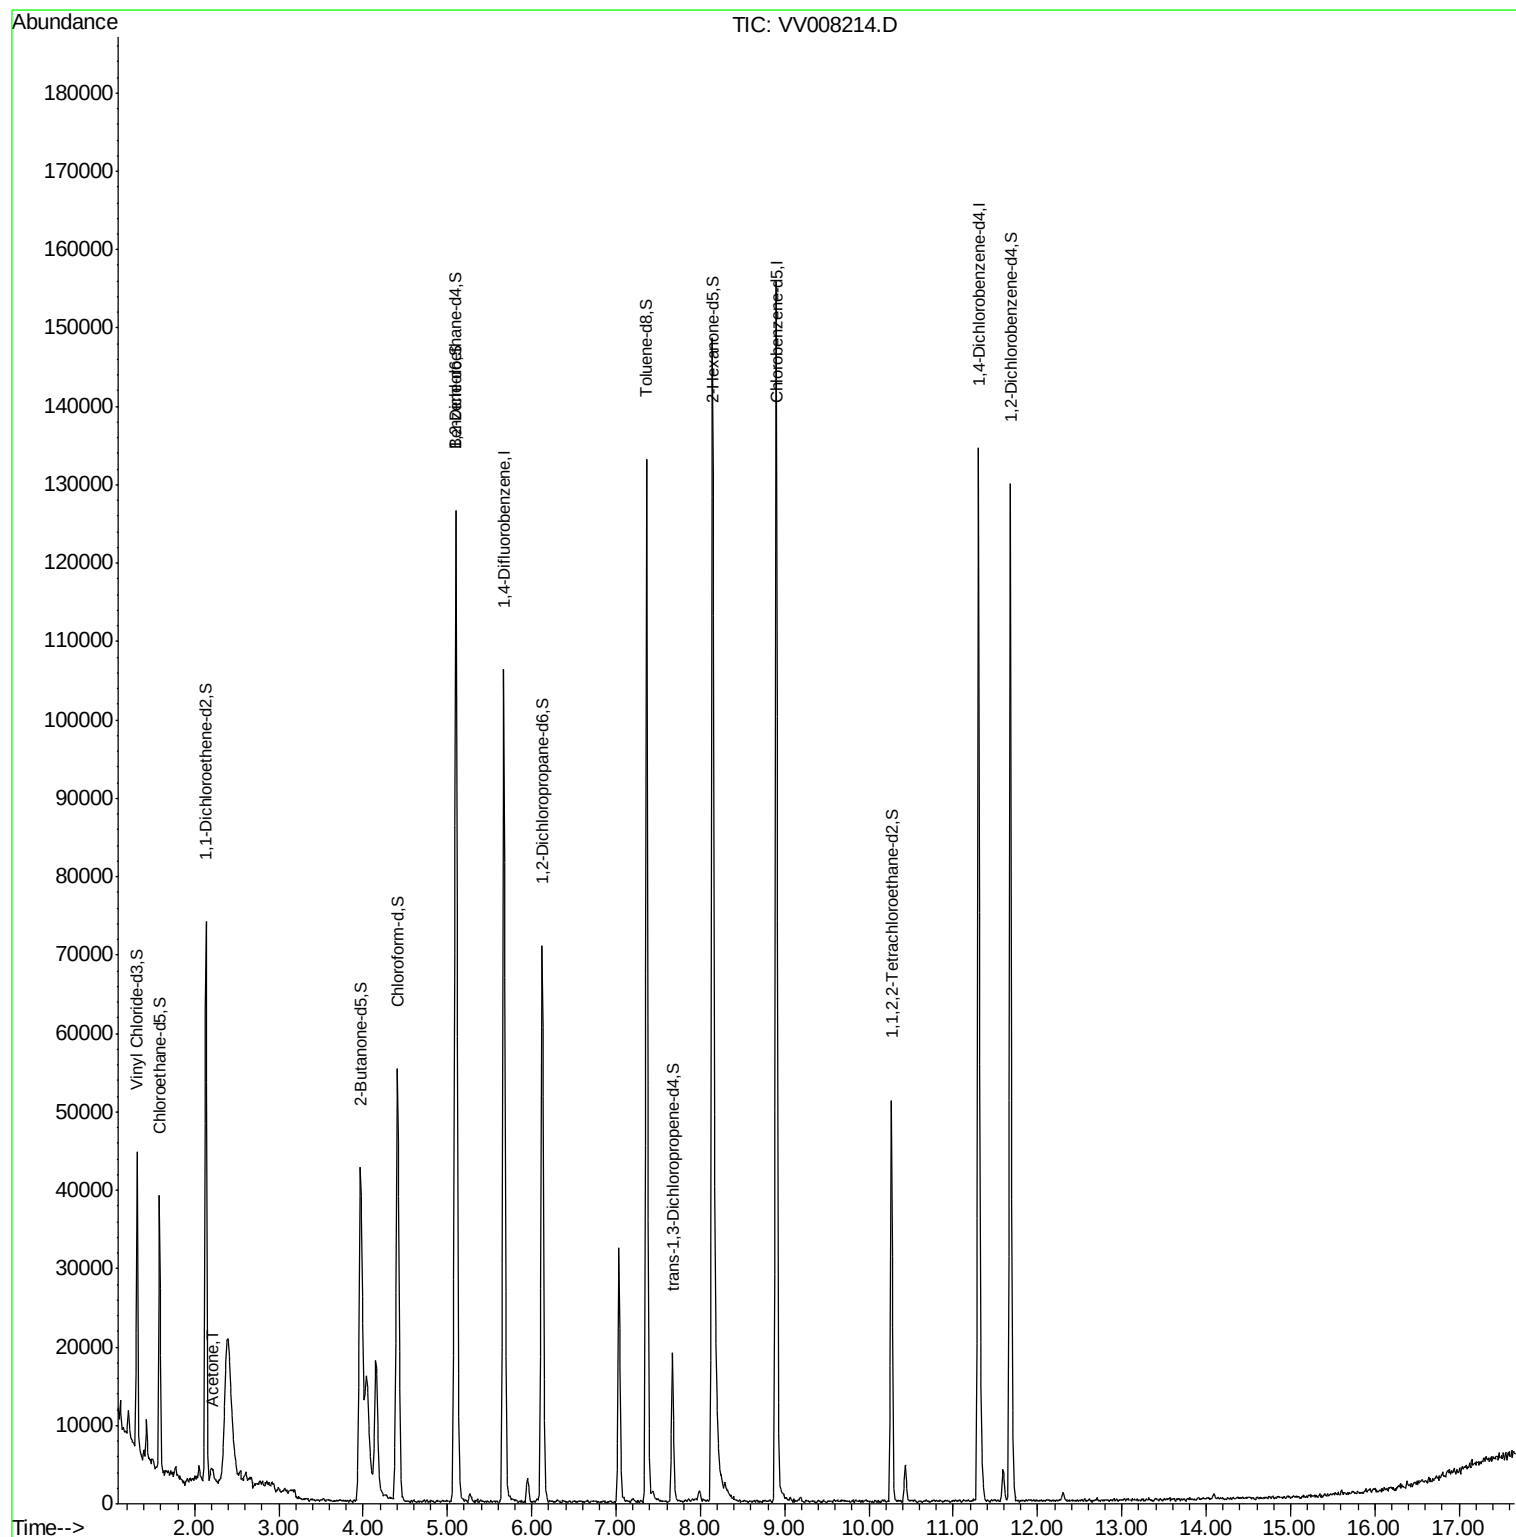

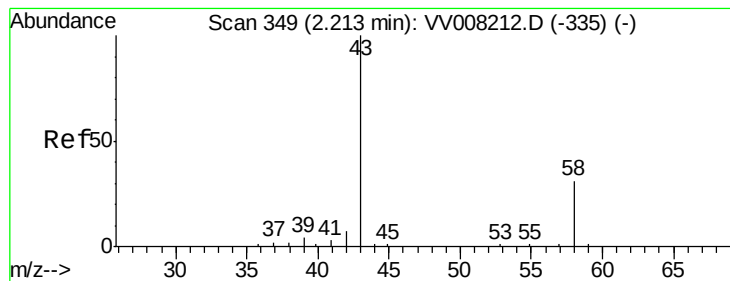

#13
 Acetone
 Concen: 2.459 ug/L
 RT: 2.22 min Scan# 351
 Delta R.T. 0.01 min
 Lab File: VV008214.D
 Acq: 09 Oct 2018 22:21

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYN1

Tot Ion: 43 Resp: 2252
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 62.2

