

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
 Data File : VV008193.D
 Acq On : 09 Oct 2018 11:18
 Operator : SY/MD
 Sample : J5280-13DL 5X
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYKODL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.216	34	39	49	rVB2	9066	8789	3.25%	0.354%
2	1.319	62	71	87	rVB	37318	45151	16.71%	1.817%
3	1.585	147	154	165	rVB	33095	35825	13.26%	1.442%
4	2.132	315	324	336	rBV	64205	93017	34.43%	3.743%
5	3.965	878	894	930	rBV2	29283	96192	35.61%	3.871%
6	4.405	1012	1031	1050	rBV2	46730	111704	41.35%	4.495%
7	5.097	1230	1246	1269	rBV2	108556	250012	92.54%	10.060%
8	5.666	1408	1423	1444	rBV	112417	220465	81.61%	8.871%
9	5.961	1502	1515	1539	rBV	124056	236889	87.69%	9.532%
10	6.122	1552	1565	1583	rBV2	60861	121766	45.07%	4.900%
11	7.032	1837	1848	1863	rBV3	27319	48815	18.07%	1.964%
12	7.363	1938	1951	1969	rBV	119420	205505	76.07%	8.269%
13	7.669	2035	2046	2060	rBV2	16587	27753	10.27%	1.117%
14	8.145	2180	2194	2228	rBV2	96432	224334	83.04%	9.027%
15	8.900	2417	2429	2456	rBV	162035	270159	100.00%	10.871%
16	10.267	2843	2854	2867	rBV	39467	62096	22.98%	2.499%
17	10.431	2892	2905	2914	rBV3	2493	4491	1.66%	0.181%
18	11.299	3164	3175	3202	rVB	139528	241986	89.57%	9.737%
19	11.678	3280	3293	3313	rBV	107050	180228	66.71%	7.252%


Sum of corrected areas: 2485177

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100918\
Data File : VV008193.D
Acq On : 09 Oct 2018 11:18
Operator : SY/MD
Sample : J5280-13DL 5X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYKODL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

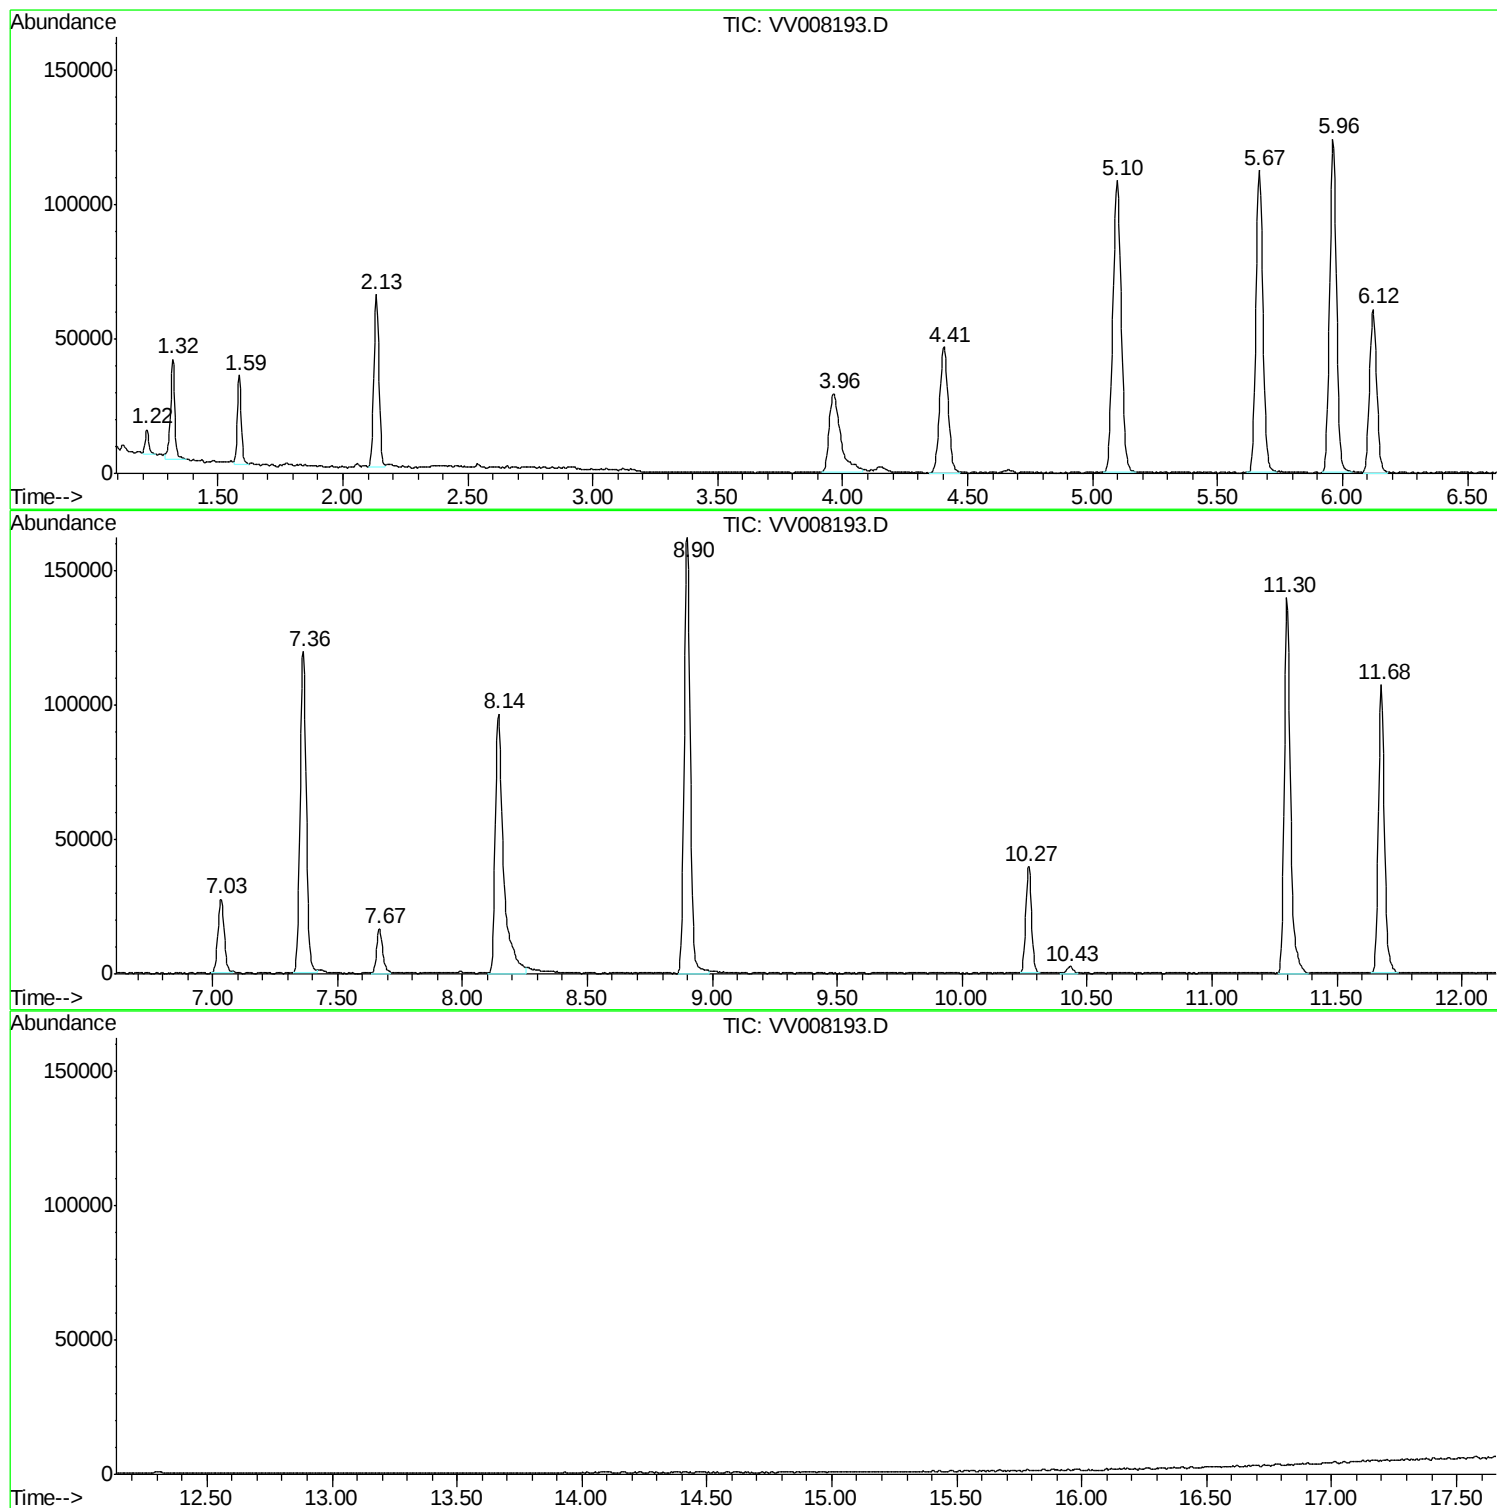

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100918\
Data File : VV008193.D
Acq On : 09 Oct 2018 11:18
Operator : SY/MD
Sample : J5280-13DL 5X
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYKODL










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	1.11 ug/L	48815	1,4-Difluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclohexadiene	80	C6H8	000592-57-4	43
2			Thiophosgene	114	CCl2S	000463-71-8	38
3			Methane, oxvbis[chloro-	114	C2H4Cl2O	000542-88-1	25
4			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
5			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25

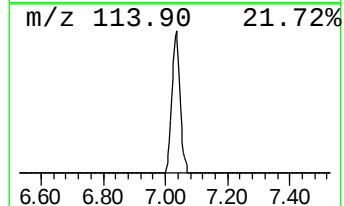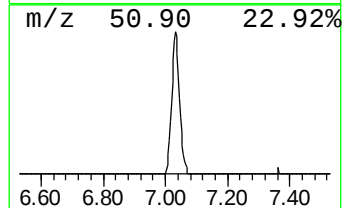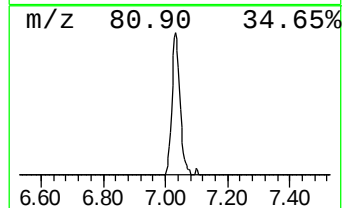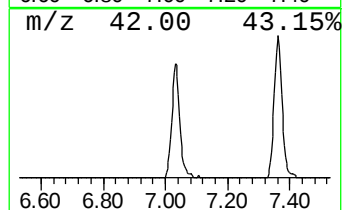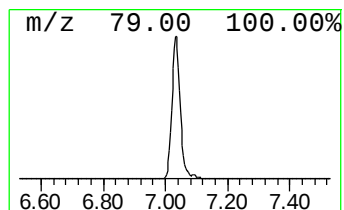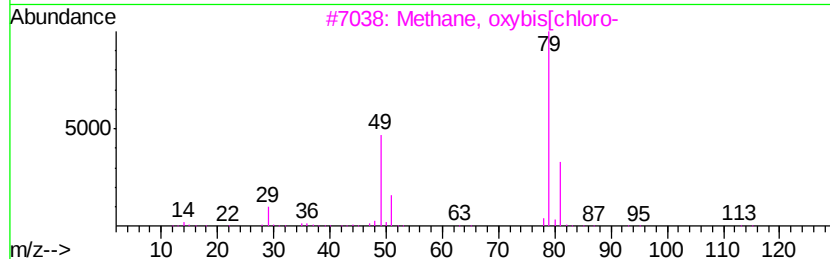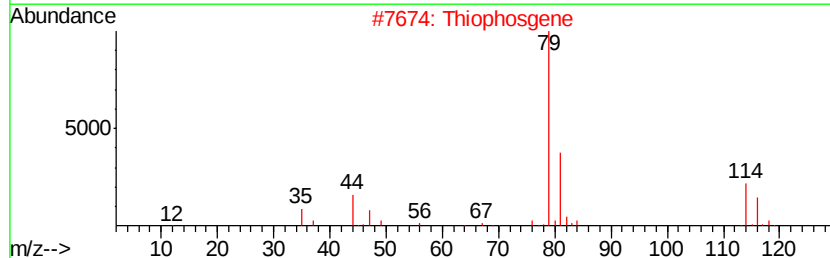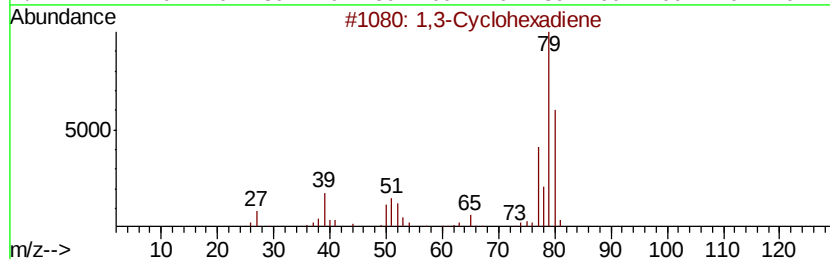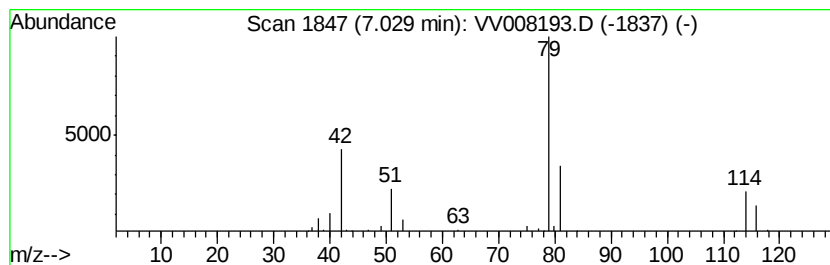

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100918\
Data File : VV008193.D
Acq On : 09 Oct 2018 11:18
Operator : SY/MD
Sample : J5280-13DL 5X
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYK0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.03	1.1	ug/L	48815	1	5.67	220465	5.0