


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100918\
 Data File : VV008190.D
 Acq On : 09 Oct 2018 09:29
 Operator : SY/MD
 Sample : BFB84
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 10 04:51:19 2018

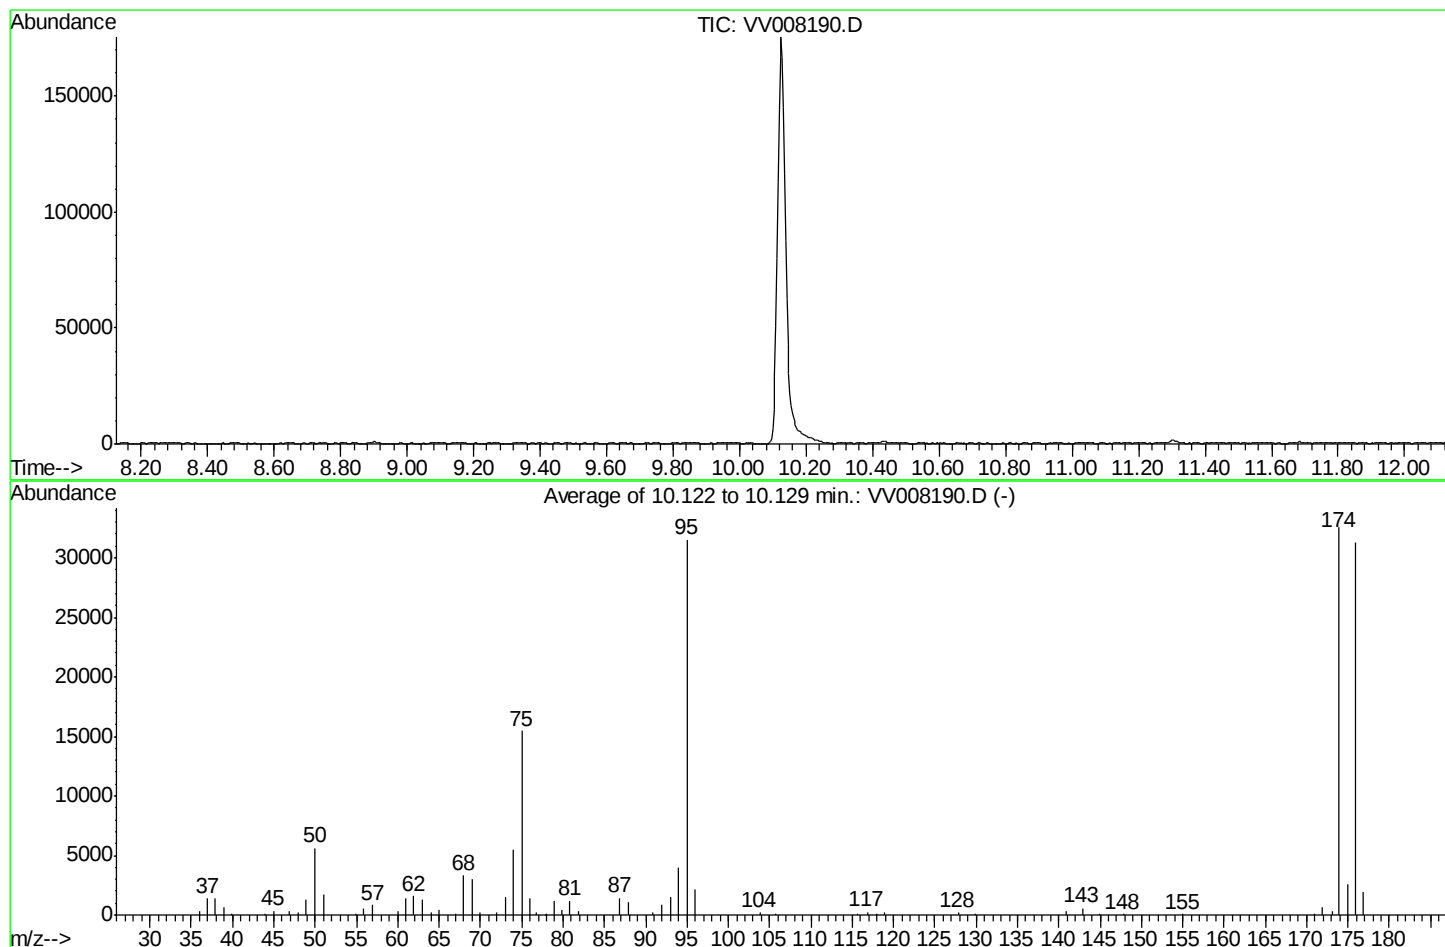

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	5626	PASS
75	95	30	80	49.0	15459	PASS
95	95	100	100	100.0	31557	PASS
96	95	5	9	6.7	2117	PASS
173	174	0.00	2	1.1	359	PASS
174	95	50	120	103.2	32568	PASS
175	174	5	9	7.9	2582	PASS
176	174	95	101	96.1	31282	PASS
177	176	5	9	6.3	1976	PASS

m/z	Abundance
43.90	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	279.0
37.00	1371.0
37.90	1340.0
38.90	662.0
40.00	123.0
43.90	426.0
45.00	327.0
46.90	334.0
47.90	226.0
48.90	1339.0
50.00	5515.0
51.00	1798.0
54.90	124.0
55.90	494.0
56.90	818.0
59.90	332.0
60.90	1409.0
62.00	1570.0
63.00	1262.0
64.00	199.0
65.00	374.0
67.00	112.0
68.00	3304.0
69.00	3009.0
69.90	249.0
72.00	191.0
73.00	1497.0
74.00	5667.0
75.00	15739.0
76.00	1443.0
76.80	188.0
77.80	129.0
78.10	147.0
78.90	1238.0
79.80	465.0
80.80	1208.0
81.90	322.0
86.90	1398.0
87.90	1171.0
90.80	166.0
92.00	884.0
92.90	1509.0
94.00	4102.0
95.00	31096.0
96.00	2133.0
103.80	141.0
105.80	145.0
116.80	235.0
117.90	115.0
118.90	257.0
127.80	167.0
129.80	151.0
140.90	318.0
142.80	560.0
144.90	165.0
147.80	126.0
170.90	128.0
171.90	579.0
173.10	508.0
173.90	31216.0
174.90	2560.0
175.90	30112.0
176.90	1964.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	292.0
37.00	1434.0
37.90	1409.0
39.00	706.0
40.00	131.0
43.80	417.0
44.90	350.0
46.90	376.0
47.90	219.0
48.90	1390.0
50.00	5792.0
51.00	1791.0
54.90	134.0
55.90	526.0
56.90	879.0
60.00	344.0
60.90	1430.0
61.90	1697.0
62.90	1305.0
64.10	188.0
65.00	417.0
67.00	157.0
68.00	3479.0
69.00	3154.0
69.90	271.0
72.00	206.0
73.00	1526.0
74.00	5753.0
75.00	15869.0
76.00	1434.0
76.80	200.0
78.10	173.0
78.90	1237.0
79.80	417.0
80.80	1251.0
81.90	352.0
86.90	1437.0
87.90	1145.0
90.80	181.0
92.00	922.0
93.00	1572.0
94.00	4103.0
95.00	32480.0
96.00	2174.0
103.80	174.0
105.80	162.0
115.70	111.0
116.80	242.0
117.90	136.0
118.90	231.0
127.80	176.0
129.90	149.0
140.90	336.0
142.90	574.0
144.90	168.0
147.80	113.0
155.00	115.0
170.90	130.0
171.80	647.0
173.10	570.0
173.90	33720.0
174.90	2668.0
175.90	32392.0
176.90	1999.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	269.0
37.00	1372.0
38.00	1327.0
39.00	702.0
39.90	130.0
43.80	402.0
44.90	318.0
46.90	369.0
48.00	202.0
48.90	1268.0
50.00	5573.0
51.00	1658.0
54.90	120.0
55.90	500.0
57.00	865.0
59.90	319.0
61.00	1360.0
61.90	1567.0
62.90	1248.0
64.10	184.0
65.00	388.0
67.00	149.0
68.00	3218.0
69.00	3040.0
69.90	270.0
72.00	202.0
73.00	1401.0
74.00	5200.0
75.00	14770.0
76.00	1318.0
76.80	200.0
78.00	138.0
78.90	1114.0
79.80	357.0
80.80	1155.0
81.90	349.0
86.90	1381.0
87.90	1069.0
90.80	181.0
92.00	899.0
93.00	1476.0
94.00	3665.0
95.00	31096.0
96.00	2044.0
103.80	188.0
105.80	184.0
115.70	111.0
116.80	233.0
117.90	165.0
118.90	212.0
127.80	170.0
129.80	124.0
141.00	345.0
142.90	523.0
144.90	150.0
155.00	133.0
171.80	639.0
173.90	32768.0
174.90	2520.0
175.90	31344.0
176.90	1967.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84