


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100919\
Data File : VV013064.D
Acq On : 09 Oct 2019 08:49
Operator : SY/MD
Sample : BFB69
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB69

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Title : VOC Analysis
Last Update : Fri Oct 11 01:36:34 2019

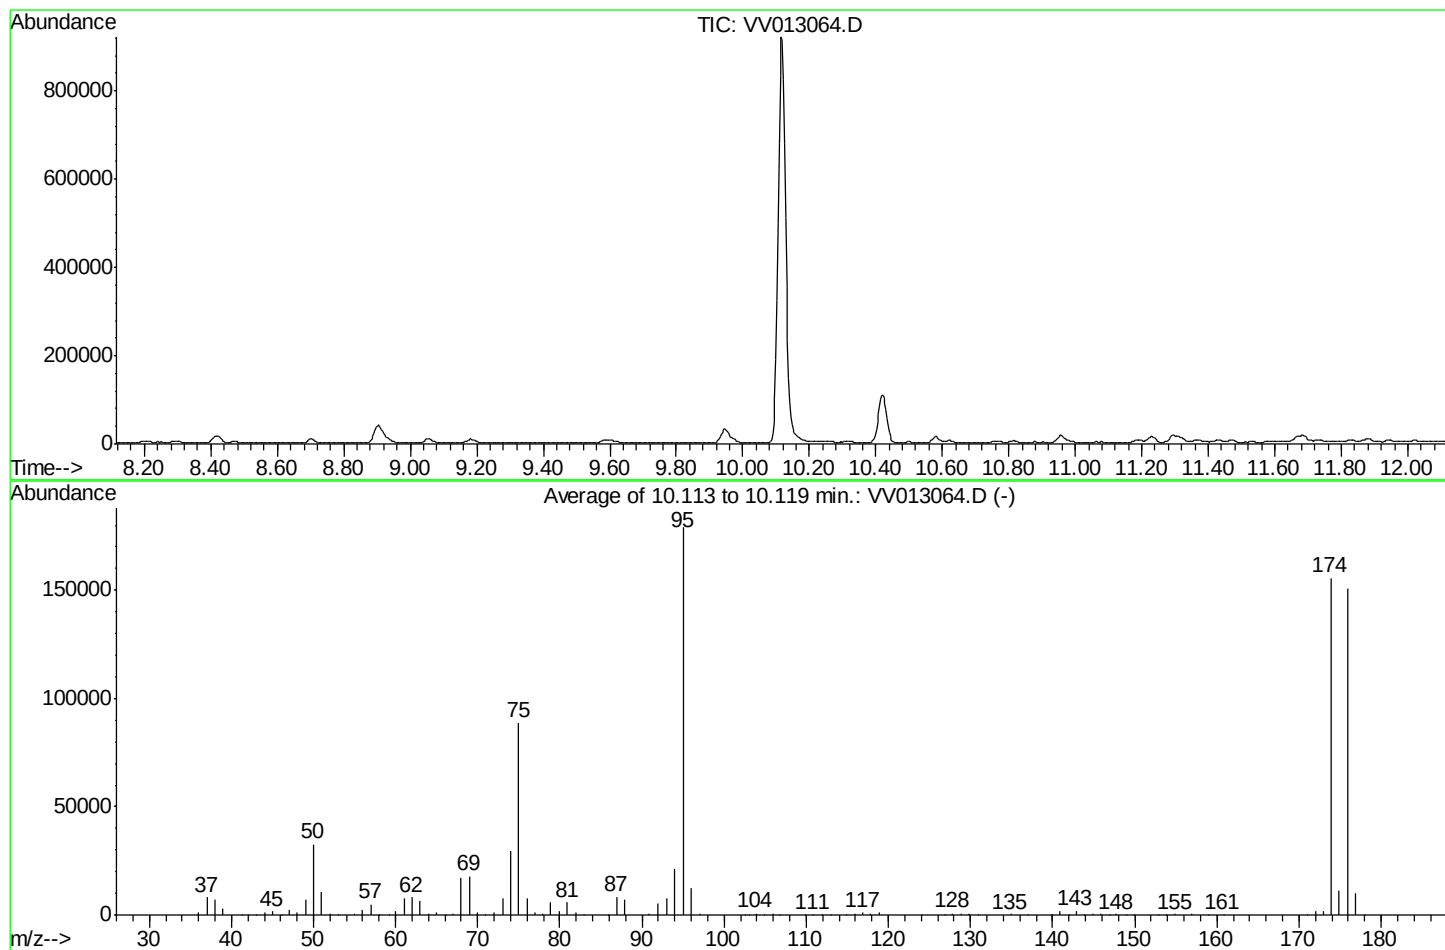

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	32805	PASS
75	95	30	80	49.6	88848	PASS
95	95	100	100	100.0	179050	PASS
96	95	5	9	6.9	12403	PASS
173	174	0.00	2	1.1	1775	PASS
174	95	50	120	87.0	155776	PASS
175	174	5	9	7.3	11362	PASS
176	174	95	101	96.6	150549	PASS
177	176	5	9	6.7	10023	PASS

Scan 2794 (10.074 min): VV013064.D
BFB69

m/z	Abundance
36.00	149.0
38.10	111.0
39.00	111.0
39.90	1215.0
43.00	162.0
44.00	1006.0
55.10	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	1507.0
37.00	7959.0
38.00	7019.0
39.00	2930.0
39.90	1121.0
42.10	148.0
43.00	168.0
44.00	1967.0
45.00	1549.0
46.00	308.0
47.00	2253.0
48.00	1283.0
49.00	6444.0
50.00	31488.0
51.00	10320.0
52.10	391.0
52.90	177.0
55.00	512.0
56.00	2259.0
57.00	4555.0
58.00	181.0
60.00	1475.0
61.00	7204.0
62.00	7946.0
63.00	6354.0
64.00	742.0
65.00	1082.0
66.10	133.0
67.00	644.0
68.00	16239.0
69.00	17000.0
70.00	1434.0
71.90	785.0
73.00	6916.0
74.00	28440.0
75.00	84144.0
76.00	7418.0
77.00	1099.0
77.90	729.0
78.90	5368.0
79.90	1455.0
80.90	5516.0
81.90	1157.0
82.80	140.0
85.80	294.0
86.90	8134.0
87.90	6582.0
90.90	557.0
92.00	4777.0
93.00	7383.0
94.00	20040.0
95.00	170112.0
96.00	11870.0
97.10	391.0
103.00	106.0
103.90	686.0
105.00	274.0
105.90	681.0
106.80	179.0
109.80	102.0
110.80	147.0
112.90	123.0
114.90	179.0
115.90	588.0
116.90	1013.0
117.80	499.0
118.90	952.0
124.00	109.0
127.80	569.0
128.80	291.0
129.80	592.0
130.90	268.0
134.90	373.0
136.90	299.0
139.80	153.0
140.90	1509.0
141.90	196.0
142.90	1911.0
143.80	132.0
144.90	407.0
145.80	402.0
147.00	166.0
147.80	408.0
149.90	194.0
152.90	179.0
153.90	170.0
155.00	360.0
156.90	340.0
159.00	219.0
160.80	298.0
171.00	216.0
172.00	1395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

173.00	1647.0
173.90	142720.0
174.90	10486.0
175.90	137536.0
176.90	9128.0
177.90	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	1532.0
37.00	8346.0
38.00	7648.0
39.00	3268.0
39.90	1167.0
41.20	103.0
42.00	137.0
43.00	228.0
44.00	2198.0
45.00	1596.0
46.10	271.0
47.00	2419.0
48.00	1287.0
49.00	7058.0
50.00	33976.0
51.00	11080.0
52.00	411.0
53.00	190.0
55.10	580.0
56.00	2466.0
57.00	4980.0
57.90	209.0
59.90	1557.0
61.00	7824.0
62.00	8575.0
63.00	6831.0
64.10	834.0
65.00	1143.0
66.00	138.0
67.00	723.0
68.00	17624.0
69.00	18480.0
70.00	1518.0
70.90	173.0
72.00	924.0
73.00	7862.0
74.00	30584.0
75.00	91720.0
76.00	7853.0
76.90	1137.0
77.90	705.0
78.90	5977.0
79.90	1560.0
80.90	5793.0
81.90	1268.0
82.90	120.0
85.90	273.0
86.90	8741.0
88.00	7247.0
90.90	675.0
92.00	5377.0
93.00	8192.0
94.00	21880.0
95.00	185600.0
96.00	12751.0
97.10	408.0
102.50	104.0
103.00	120.0
103.90	748.0
104.80	318.0
105.90	681.0
106.80	229.0
109.80	108.0
110.90	220.0
112.90	153.0
114.90	214.0
115.90	678.0
116.90	1098.0
117.80	563.0
118.90	1037.0
126.80	103.0
127.90	675.0
128.80	376.0
129.80	650.0
131.00	265.0
134.90	436.0
137.00	325.0
140.00	169.0
140.90	1609.0
141.90	219.0
142.80	2027.0
143.90	141.0
145.00	417.0
145.80	356.0
147.00	138.0
147.80	484.0
149.00	131.0
149.90	183.0
152.90	182.0
153.90	174.0
154.90	388.0
156.90	359.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

159.00	236.0
160.80	308.0
171.00	187.0
172.00	1582.0
173.00	1816.0
173.90	160832.0
174.90	11657.0
175.90	155712.0
176.90	10529.0
178.00	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	1427.0
37.00	7865.0
38.00	7253.0
39.00	3165.0
40.00	1138.0
41.90	113.0
43.00	281.0
44.00	2144.0
45.00	1505.0
46.20	208.0
47.00	2247.0
48.00	1119.0
49.00	6971.0
50.00	32952.0
51.00	10832.0
52.00	395.0
53.10	205.0
55.10	533.0
56.00	2535.0
57.00	4927.0
57.90	267.0
59.20	117.0
59.90	1501.0
61.00	7929.0
62.00	8193.0
63.00	6828.0
64.10	852.0
65.00	1052.0
66.00	162.0
67.00	687.0
68.00	17496.0
69.00	18248.0
70.00	1480.0
70.90	224.0
72.00	1032.0
73.00	7934.0
74.00	30128.0
75.00	90680.0
76.00	7656.0
76.90	1211.0
78.00	661.0
78.90	5739.0
79.90	1539.0
80.90	5612.0
82.00	1233.0
83.00	108.0
86.00	214.0
86.90	8254.0
88.00	7385.0
90.90	670.0
92.00	5335.0
93.00	8119.0
94.00	21560.0
95.00	181440.0
96.00	12588.0
97.00	450.0
103.10	117.0
103.90	731.0
104.80	345.0
105.90	653.0
106.80	232.0
110.90	258.0
111.90	106.0
112.90	183.0
114.80	211.0
115.90	744.0
116.90	1027.0
117.80	585.0
118.90	1017.0
126.80	140.0
127.90	730.0
128.80	421.0
129.90	643.0
131.00	253.0
134.90	377.0
136.90	305.0
139.90	159.0
140.90	1628.0
141.90	248.0
142.90	1945.0
143.90	135.0
145.00	450.0
145.80	279.0
146.90	135.0
147.80	484.0
149.00	154.0
149.90	154.0
152.90	132.0
153.80	181.0
154.90	414.0
156.90	346.0
158.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

160.80	232.0
171.00	149.0
172.00	1639.0
173.00	1863.0
173.90	163776.0
174.90	11944.0
175.90	158400.0
176.90	10412.0
178.00	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69