
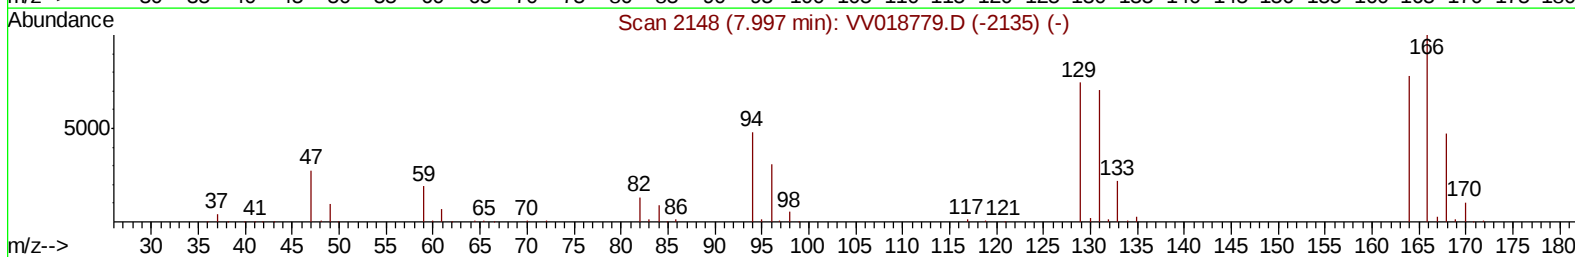
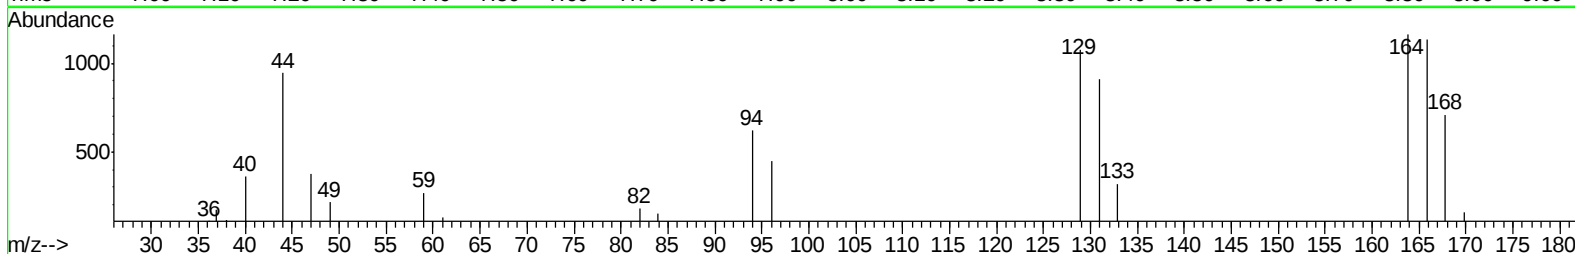


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100920\
Data File : VV018783.D
Acq On : 09 Oct 2020 00:38
Operator : SY/MD
Sample : L4239-09DL 400X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Oct 09 07:32:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 09 07:31:27 2020
Response via : Initial Calibration

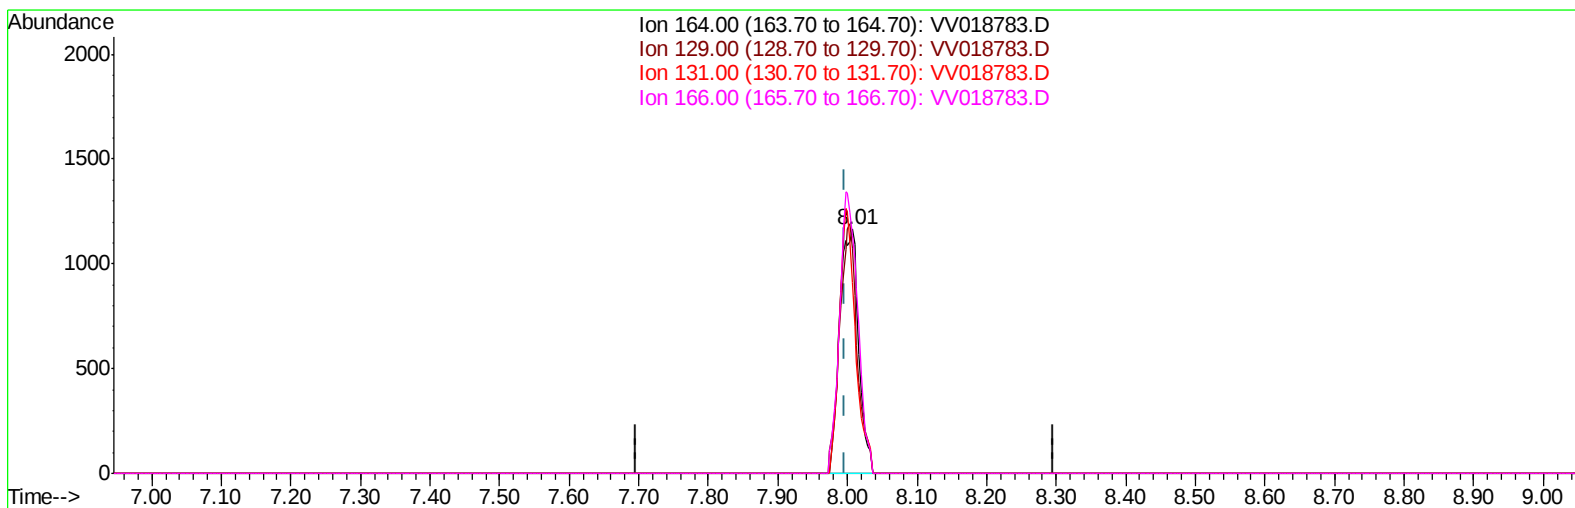

TIC: VV018783.D

(46) Tetrachloroethene (T)

8.007min (+0.010) 1.11ug/L m

response 2204

Ion	Exp%	Act%
164.00	100	100
129.00	92.30	92.27
131.00	90.80	78.44
166.00	126.20	97.59