

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100920\
 Data File : VV018814.D
 Acq On : 09 Oct 2020 13:15
 Operator : SY/MD
 Sample : L4239-16 4X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3R9

Quant Time: Oct 10 01:39:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 09 23:43:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	377802	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	371244	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	174572	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	130112	37.90	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.80%
7) Chloroethane-d5	1.58	69	115388	41.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.52%
11) 1,1-Dichloroethene-d2	2.12	63	198364	29.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.94%#
21) 2-Butanone-d5	3.91	46	210901	100.06	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.06%
24) Chloroform-d	4.38	84	241407	39.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.72%
26) 1,2-Dichloroethane-d4	5.06	65	174414	42.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.96%
32) Benzene-d6	5.07	84	496991	41.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.20%
36) 1,2-Dichloropropane-d6	6.09	67	163990	42.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.20%
41) Toluene-d8	7.34	98	415414	39.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.34%#
43) trans-1,3-Dichloropropene-	7.64	79	73931	38.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.64%
47) 2-Hexanone-d5	8.11	63	111646	81.77	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.77%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	172173	38.42	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.84%
64) 1,2-Dichlorobenzene-d4	11.65	152	175107	45.32	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.64%

Target Compounds


					Ovalue
51) Chlorobenzene	8.90	112	1353638	168.588	ug/L 99
62) 1,3-Dichlorobenzene	11.20	146	131881	23.172	ug/L 98
63) 1,4-Dichlorobenzene	11.29	146	268525	45.356	ug/L 100
65) 1,2-Dichlorobenzene	11.66	146	3787	0.663	ug/L # 79
68) 1,2,4-trichlorobenzene	13.29	180	10837	3.126	ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100920\
Data File : VV018814.D
Acq On : 09 Oct 2020 13:15
Operator : SY/MD
Sample : L4239-16 4X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3R9

Quant Time: Oct 10 01:39:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 09 23:43:53 2020
Response via : Initial Calibration

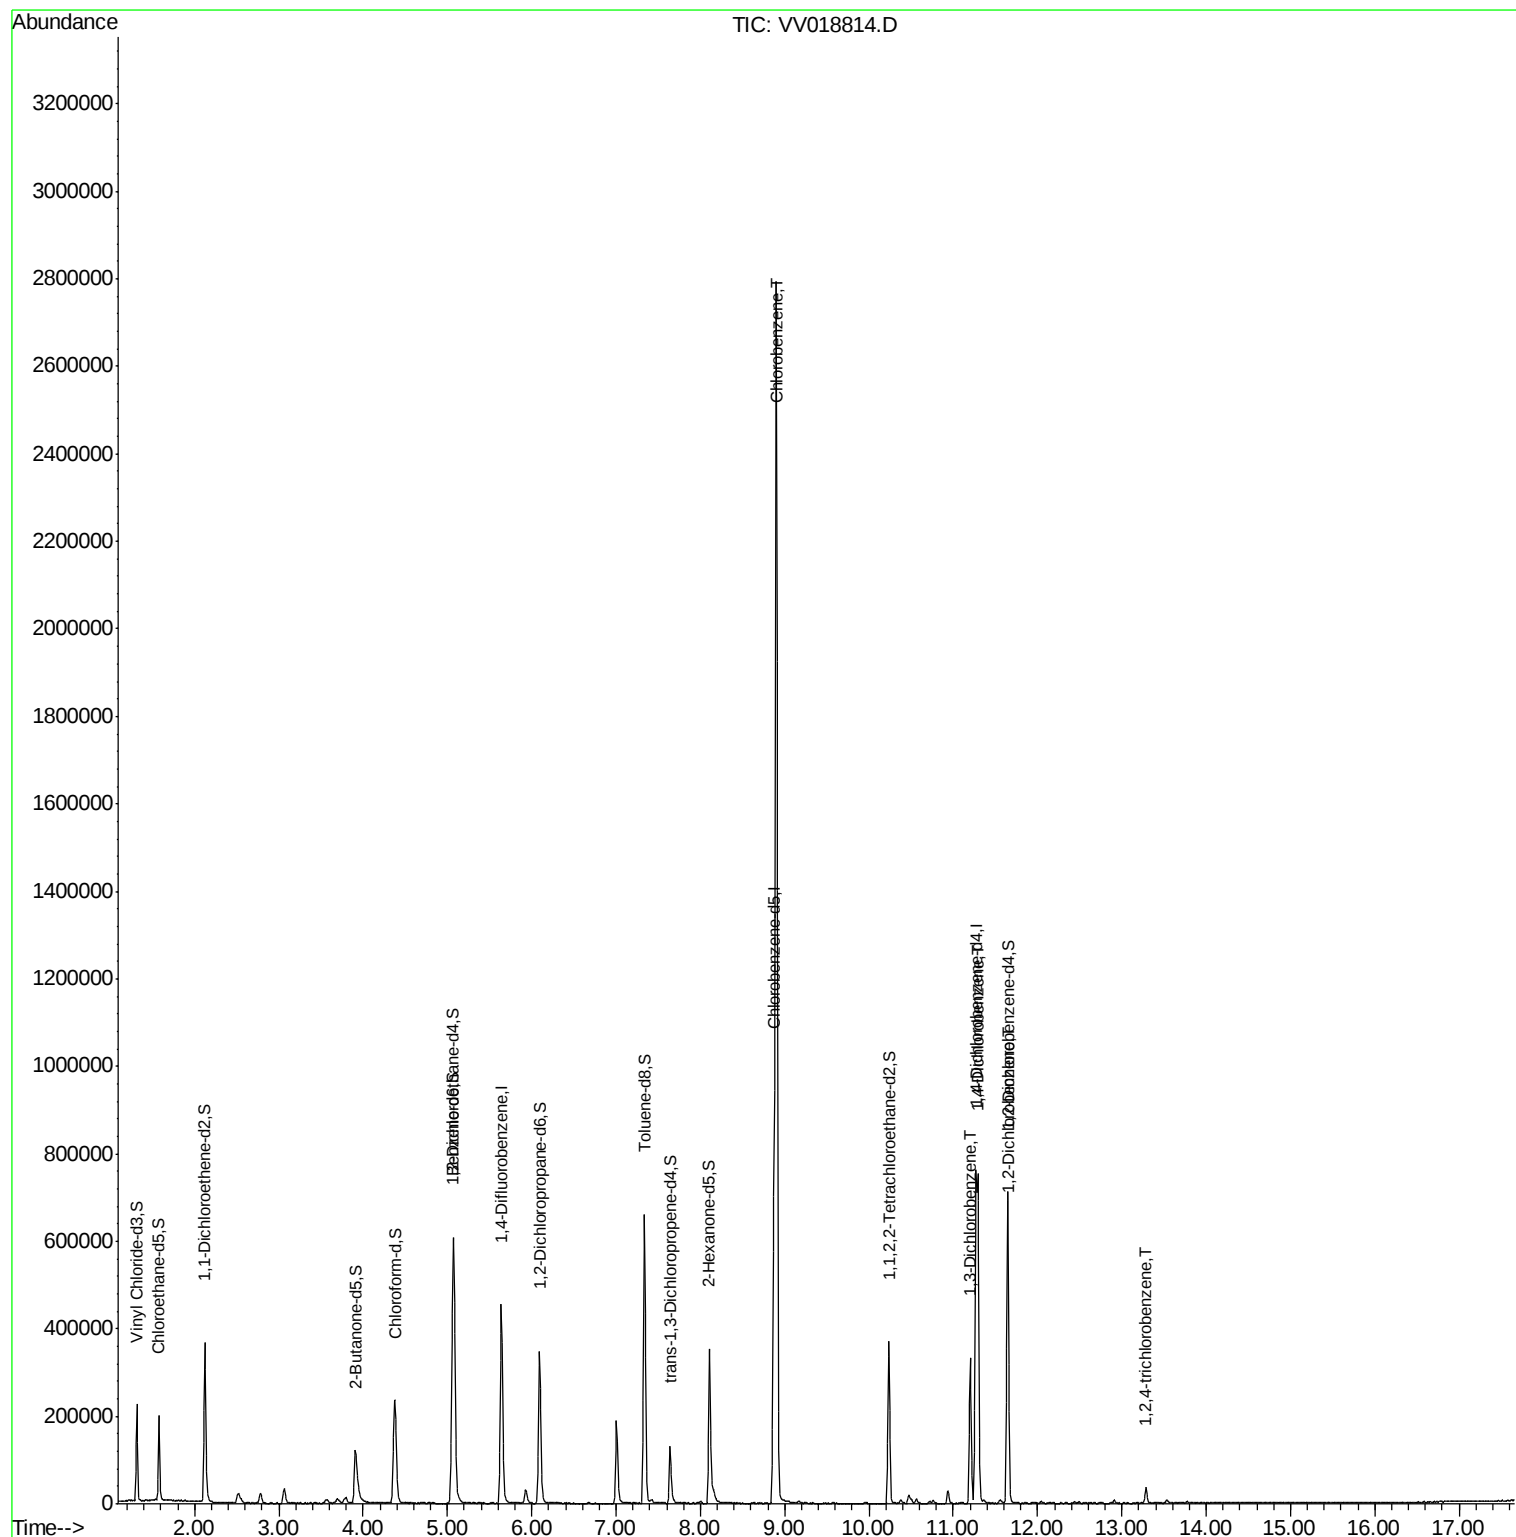

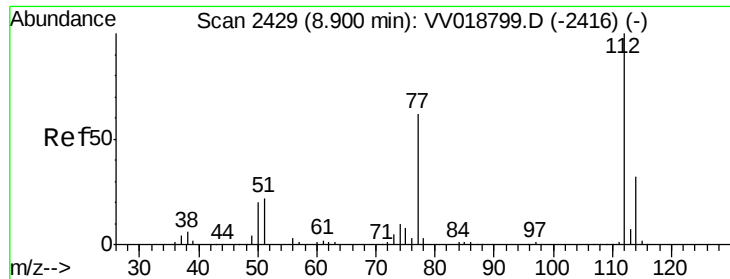

#51

Chlorobenzene

Concen: 168.588 ug/L

RT: 8.90 min Scan# 2429

Delta R.T. 0.00 min

Lab File: VV018814.D

Acq: 09 Oct 2020 13:15

Instrument :

MSVOA_V

ClientSampled :

BG3R9


Tot Ion:112 Resp: 1353638

Ion Ratio Lower Upper

112 100

114 32.5 22.0 41.0




77 62.3 49.8 74.6

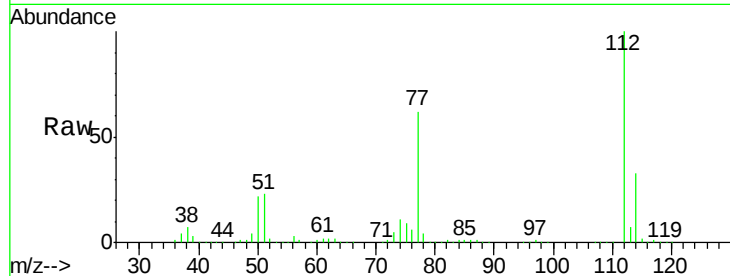

Abundance Ion 112.00 (111.70 to 112.70): V

Ion 114.00 (113.70 to 114.70): V

Ion 77.00 (76.70 to 77.70): V

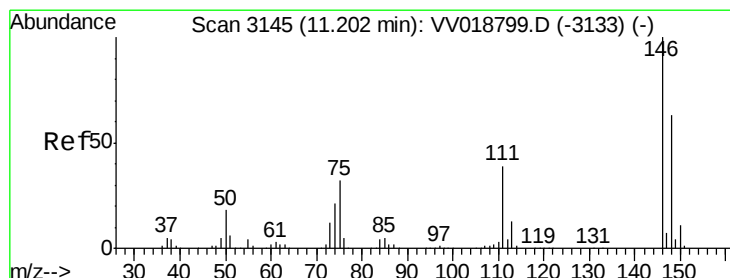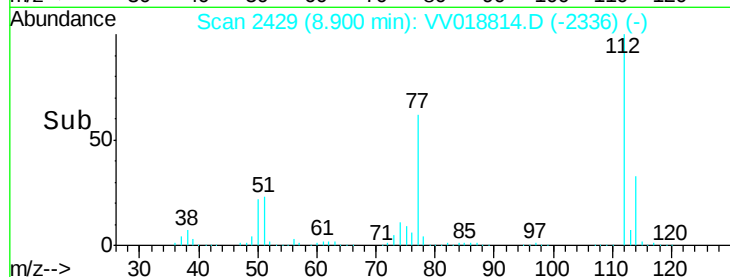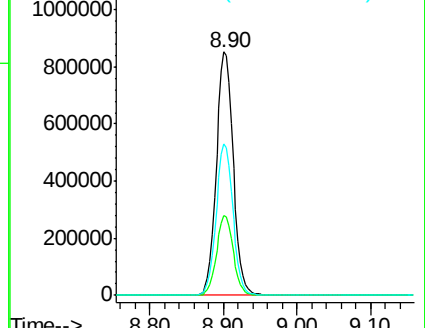

#62

1,3-Dichlorobenzene

Concen: 23.172 ug/L

RT: 11.20 min Scan# 3145

Delta R.T. 0.00 min

Lab File: VV018814.D

Acq: 09 Oct 2020 13:15


Tgt Ion:146 Resp: 131881

Ion Ratio Lower Upper

146 100

111 38.2 27.8 51.6



148 63.7 45.4 84.4

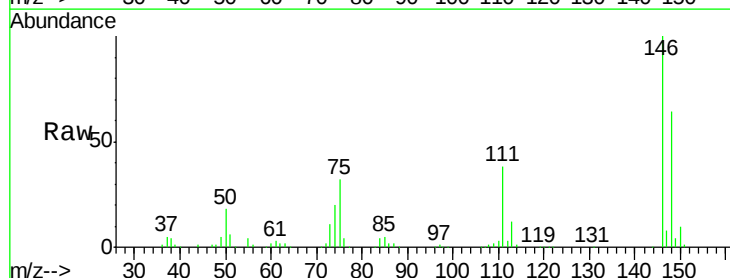


Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

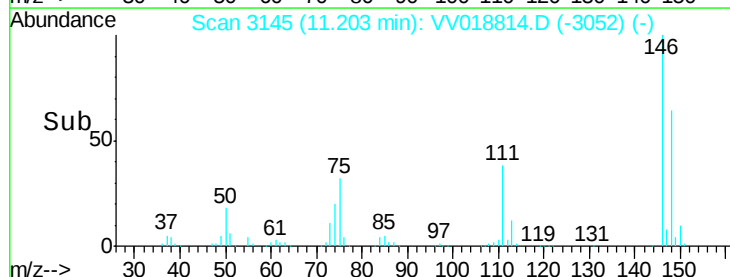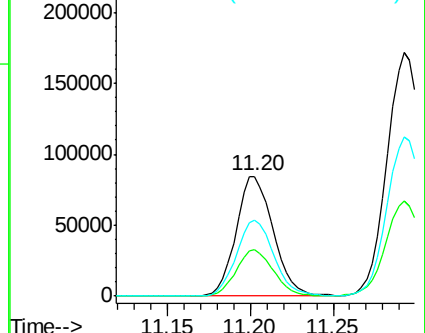

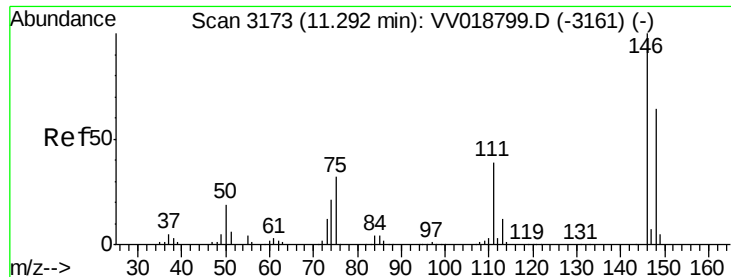

#63

1,4-Dichlorobenzene

Concen: 45.356 ug/L

RT: 11.29 min Scan# 3173

Delta R.T. 0.00 min

Lab File: VV018814.D

Acq: 09 Oct 2020 13:15

Instrument :

MSVOA_V

ClientSampled :

BG3R9


Tot Ion:146 Resp: 268525

Ion Ratio Lower Upper

146 100

111 38.9 27.1 50.3




148 65.3 45.4 84.4

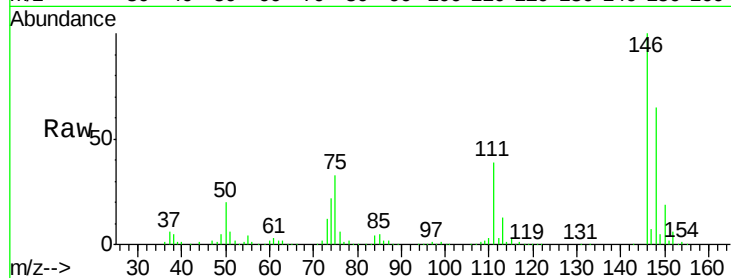

Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

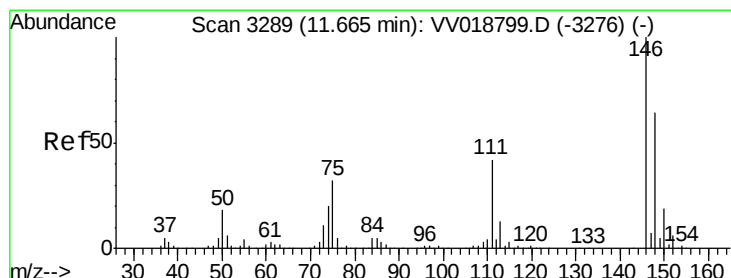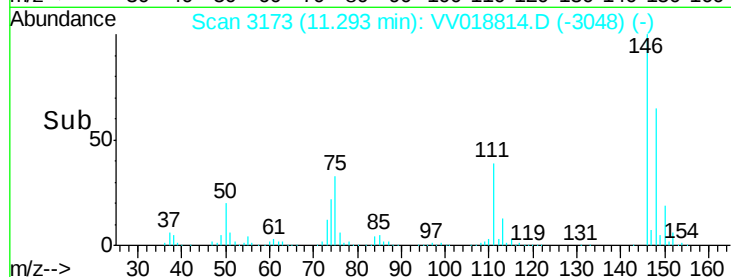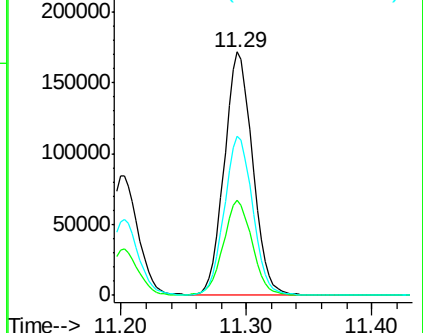

#65

1,2-Dichlorobenzene

Concen: 0.663 ug/L

RT: 11.66 min Scan# 3288

Delta R.T. -0.00 min

Lab File: VV018814.D

Acq: 09 Oct 2020 13:15


Tgt Ion:146 Resp: 3787

Ion Ratio Lower Upper

146 100

111 61.2 33.8 50.6#



148 75.0 50.3 75.5

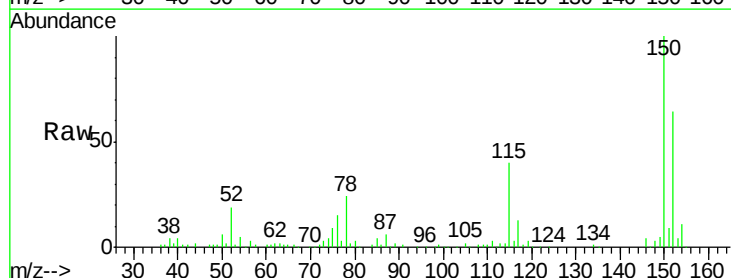


Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

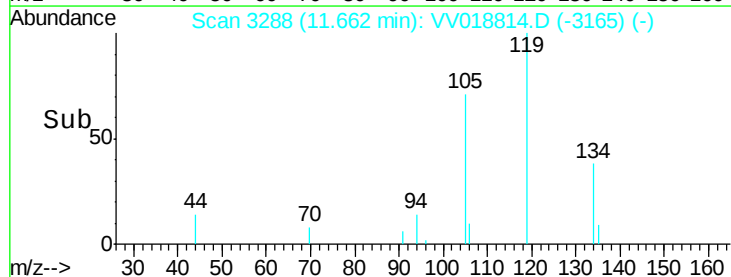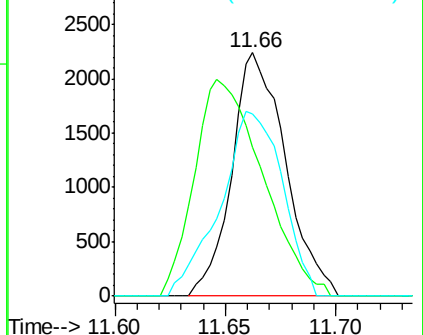


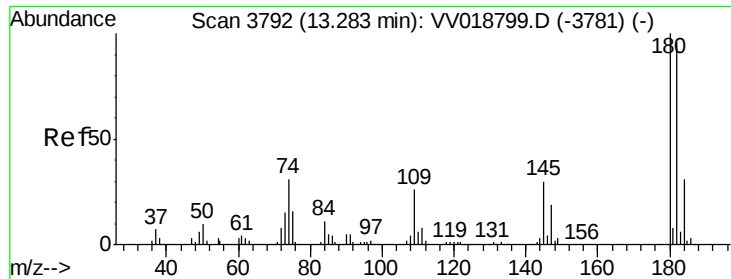

#68
 1,2,4-trichlorobenzene
 Concen: 3.126 ug/L
 RT: 13.29 min Scan# 3793
 Delta R.T. 0.00 min
 Lab File: VV018814.D
 Acq: 09 Oct 2020 13:15

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3R9

Tot Ion:180 Resp: 10837
 Ion Ratio Lower Upper
 180 100
 182 95.4 76.7 115.1
 145 31.4 24.0 36.0

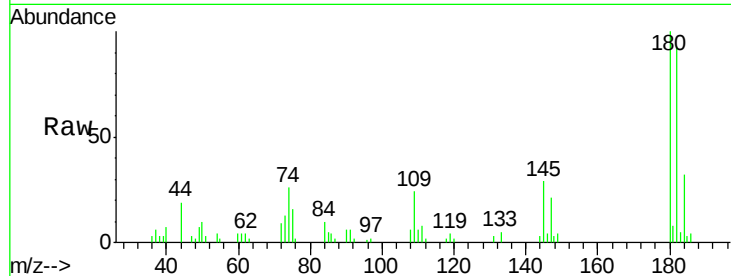

Abundance Ion 180.00 (179.70 to 180.70): V
 Ion 182.00 (181.70 to 182.70): V
 Ion 145.00 (144.70 to 145.70): V

