

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100920\
 Data File : VV018790.D
 Acq On : 09 Oct 2020 03:24
 Operator : SY/MD
 Sample : L4239-18DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	224361	221019	14.01%	1.775%
2	1.576	144	151	165	rVB	189128	212675	13.48%	1.708%
3	2.123	311	321	349	rVB	363767	561769	35.61%	4.513%
4	2.782	514	526	542	rVB2	9825	20518	1.30%	0.165%
5	2.881	553	557	561	rBV3	491	484	0.03%	0.004%
6	3.016	596	599	602	rVB	401	247	0.02%	0.002%
7	3.065	602	614	628	rBV6	2143	5398	0.34%	0.043%
8	3.119	628	631	636	rVB4	695	563	0.04%	0.005%
9	3.145	636	639	643	rBV2	300	237	0.02%	0.002%
10	3.251	665	672	674	rBV2	389	366	0.02%	0.003%
11	3.393	714	716	717	rBV2	395	141	0.01%	0.001%
12	3.415	721	723	725	rVB2	215	92	0.01%	0.001%
13	3.434	725	729	733	rBV2	459	459	0.03%	0.004%
14	3.566	756	770	787	rVB3	6915	18591	1.18%	0.149%
15	3.637	787	792	793	rBV2	549	348	0.02%	0.003%
16	3.846	854	857	859	rBV2	253	156	0.01%	0.001%
17	3.865	859	863	864	rBV2	326	264	0.02%	0.002%
18	3.901	864	874	913	rBV	117624	329261	20.87%	2.645%
19	4.376	1007	1022	1051	rVB	242805	598368	37.93%	4.807%
20	4.711	1122	1126	1128	rBV3	610	574	0.04%	0.005%
21	4.901	1183	1185	1188	rBV2	328	207	0.01%	0.002%
22	5.071	1216	1238	1269	rBV2	609630	1577571	100.00%	12.672%
23	5.399	1338	1340	1342	rBV2	318	133	0.01%	0.001%
24	5.540	1383	1384	1388	rVB2	390	95	0.01%	0.001%
25	5.566	1388	1392	1394	rBV2	418	301	0.02%	0.002%
26	5.640	1402	1415	1436	rBV	417508	836355	53.02%	6.718%
27	5.929	1494	1505	1529	rVB2	44141	93729	5.94%	0.753%
28	6.093	1542	1556	1582	rBV	354361	715586	45.36%	5.748%
29	6.360	1638	1639	1641	rBV	229	114	0.01%	0.001%
30	6.418	1655	1657	1658	rBV	353	109	0.01%	0.001%
31	6.428	1658	1660	1663	rBV	296	214	0.01%	0.002%
32	6.466	1669	1672	1676	rBV3	626	424	0.03%	0.003%
33	6.544	1694	1696	1698	rBV	359	143	0.01%	0.001%
34	6.566	1701	1703	1704	rBV2	446	153	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100920\
 Data File : VV018790.D
 Acq On : 09 Oct 2020 03:24
 Operator : SY/MD
 Sample : L4239-18DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	6.753	1758	1761	1767	rVB5	600	465	0.03%	0.004%
36	6.781	1767	1770	1774	rBV2	518	457	0.03%	0.004%
37	6.814	1777	1780	1786	rBV2	405	424	0.03%	0.003%
38	6.843	1786	1789	1791	rBV2	452	301	0.02%	0.002%
39	6.923	1811	1814	1818	rBV	324	224	0.01%	0.002%
40	7.007	1828	1840	1869	rBV	187873	344936	21.87%	2.771%
41	7.338	1931	1943	1966	rBV	713878	1233259	78.17%	9.907%
42	7.643	2027	2038	2063	rBV	136830	244559	15.50%	1.965%
43	7.875	2109	2110	2113	rBV2	358	140	0.01%	0.001%
44	7.894	2113	2116	2120	rBV3	583	484	0.03%	0.004%
45	7.929	2123	2127	2129	rBV2	829	673	0.04%	0.005%
46	8.000	2141	2149	2162	rVB5	7576	13067	0.83%	0.105%
47	8.106	2172	2182	2227	rBV2	347599	707469	44.85%	5.683%
48	8.502	2303	2305	2307	rBV3	530	313	0.02%	0.003%
49	8.556	2320	2322	2325	rBV2	418	213	0.01%	0.002%
50	8.605	2335	2337	2340	rBV2	324	203	0.01%	0.002%
51	8.724	2372	2374	2378	rVB2	408	233	0.01%	0.002%
52	8.749	2380	2382	2387	rVV3	332	260	0.02%	0.002%
53	8.875	2408	2421	2424	rBV	688605	1006781	63.82%	8.087%
54	9.129	2498	2500	2502	rBV3	732	430	0.03%	0.003%
55	9.215	2525	2527	2528	rBV2	318	104	0.01%	0.001%
56	9.347	2566	2568	2575	rBV2	560	591	0.04%	0.005%
57	9.386	2577	2580	2584	rVB2	572	362	0.02%	0.003%
58	9.408	2584	2587	2590	rBV2	410	316	0.02%	0.003%
59	9.482	2607	2610	2614	rVB2	489	380	0.02%	0.003%
60	9.605	2644	2648	2650	rBV3	399	311	0.02%	0.002%
61	9.656	2660	2664	2665	rBV	239	177	0.01%	0.001%
62	9.768	2697	2699	2707	rVB2	733	489	0.03%	0.004%
63	9.810	2710	2712	2715	rBV2	269	218	0.01%	0.002%
64	9.833	2715	2719	2721	rVB	590	422	0.03%	0.003%
65	9.846	2721	2723	2725	rBV	214	107	0.01%	0.001%
66	9.958	2750	2758	2763	rBV5	1560	2018	0.13%	0.016%
67	10.051	2784	2787	2790	rBV3	371	243	0.02%	0.002%
68	10.113	2803	2806	2807	rBV	384	200	0.01%	0.002%
69	10.238	2830	2845	2862	rBV	356449	568960	36.07%	4.570%
70	10.508	2926	2929	2935	rVB2	620	525	0.03%	0.004%
71	10.598	2953	2957	2961	rBV2	419	361	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100920\
 Data File : VV018790.D
 Acq On : 09 Oct 2020 03:24
 Operator : SY/MD
 Sample : L4239-18DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	10.717	2992	2994	3003	rVB4	781	600	0.04%	0.005%
73	10.781	3013	3014	3016	rBV	343	137	0.01%	0.001%
74	10.939	3059	3063	3069	rBV4	1093	1075	0.07%	0.009%
75	11.055	3096	3099	3101	rBV	314	228	0.01%	0.002%
76	11.074	3103	3105	3107	rBV	471	277	0.02%	0.002%
77	11.203	3131	3145	3156	rBV	418699	638681	40.49%	5.130%
78	11.273	3156	3167	3169	rBV	728297	984457	62.40%	7.908%
79	11.556	3243	3255	3269	rBV4	13690	31009	1.97%	0.249%
80	11.646	3271	3283	3307	rVV	731048	1136583	72.05%	9.130%
81	11.759	3315	3318	3322	rBV4	1321	1227	0.08%	0.010%
82	12.100	3422	3424	3427	rBV2	362	234	0.01%	0.002%
83	12.231	3462	3465	3469	rBV	490	399	0.03%	0.003%
84	12.437	3524	3529	3532	rBV4	1676	1796	0.11%	0.014%
85	12.572	3567	3571	3583	rVB5	2246	2647	0.17%	0.021%
86	12.672	3595	3602	3610	rBV5	2651	4189	0.27%	0.034%
87	12.752	3621	3627	3635	rVB4	2598	3136	0.20%	0.025%
88	12.907	3668	3675	3685	rVB3	11128	15463	0.98%	0.124%
89	12.968	3692	3694	3696	rBV	429	272	0.02%	0.002%
90	13.048	3717	3719	3725	rVB2	412	322	0.02%	0.003%
91	13.135	3741	3746	3751	rBV2	541	622	0.04%	0.005%
92	13.186	3759	3762	3764	rBV2	690	483	0.03%	0.004%
93	13.283	3781	3792	3806	rBV	180628	284811	18.05%	2.288%
94	13.450	3836	3844	3845	rBV3	525	629	0.04%	0.005%
95	13.585	3883	3886	3888	rBV	387	300	0.02%	0.002%
96	13.614	3893	3895	3897	rBV	472	218	0.01%	0.002%
97	13.736	3929	3933	3940	rVB5	1372	1319	0.08%	0.011%
98	13.932	3988	3994	4000	rBV3	1483	1836	0.12%	0.015%
99	14.167	4065	4067	4072	rBV2	404	251	0.02%	0.002%
100	15.321	4422	4426	4430	rVB	13631	8294	0.53%	0.067%


Sum of corrected areas: 12448834

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100920\
Data File : VV018790.D
Acq On : 09 Oct 2020 03:24
Operator : SY/MD
Sample : L4239-18DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG3S2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

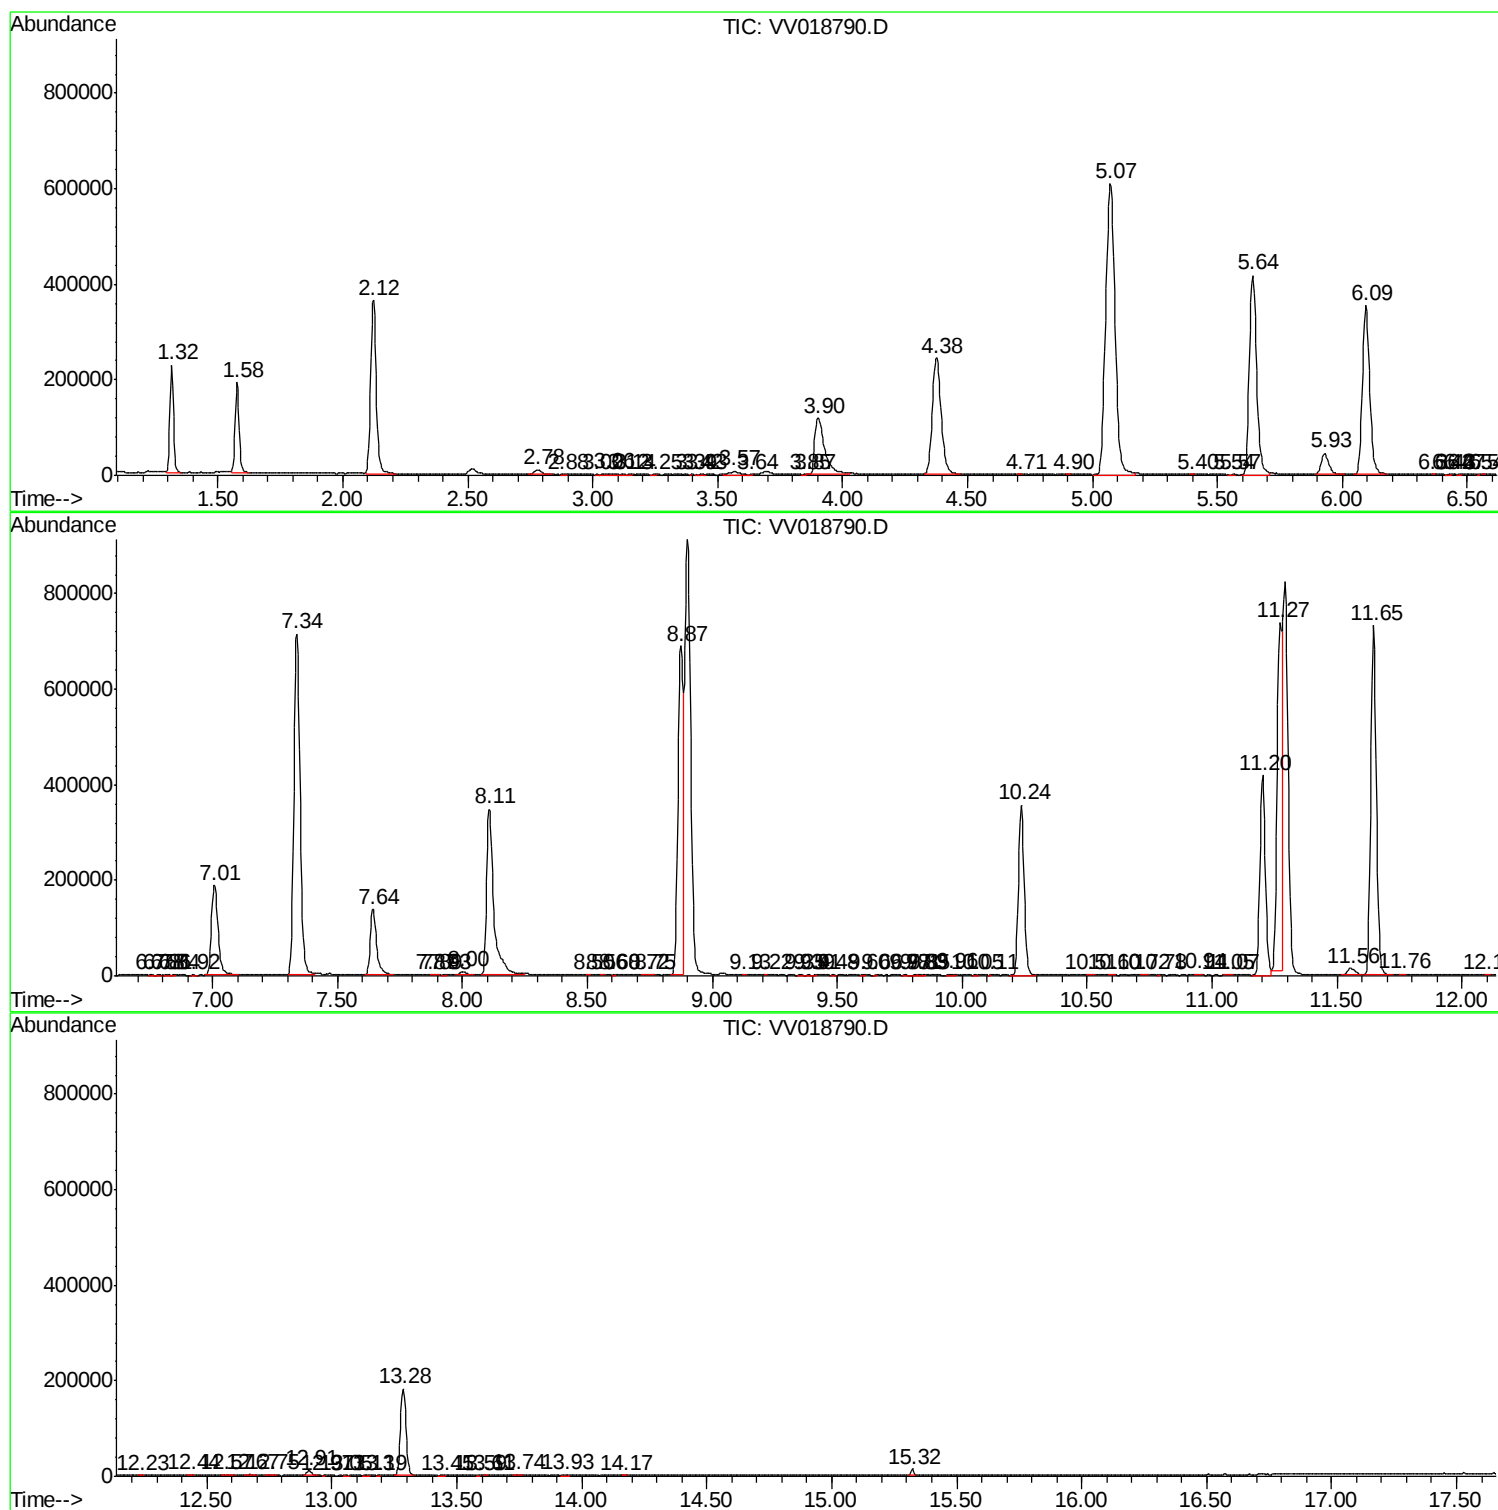

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV100920\
Data File : VV018790.D
Acq On : 09 Oct 2020 03:24
Operator : SY/MD
Sample : L4239-18DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3S2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100920\
Data File : VV018790.D
Acq On : 09 Oct 2020 03:24
Operator : SY/MD
Sample : L4239-18DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3S2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc