


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100920\
 Data File : VV018772.D
 Acq On : 08 Oct 2020 18:55
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 09 07:31:27 2020

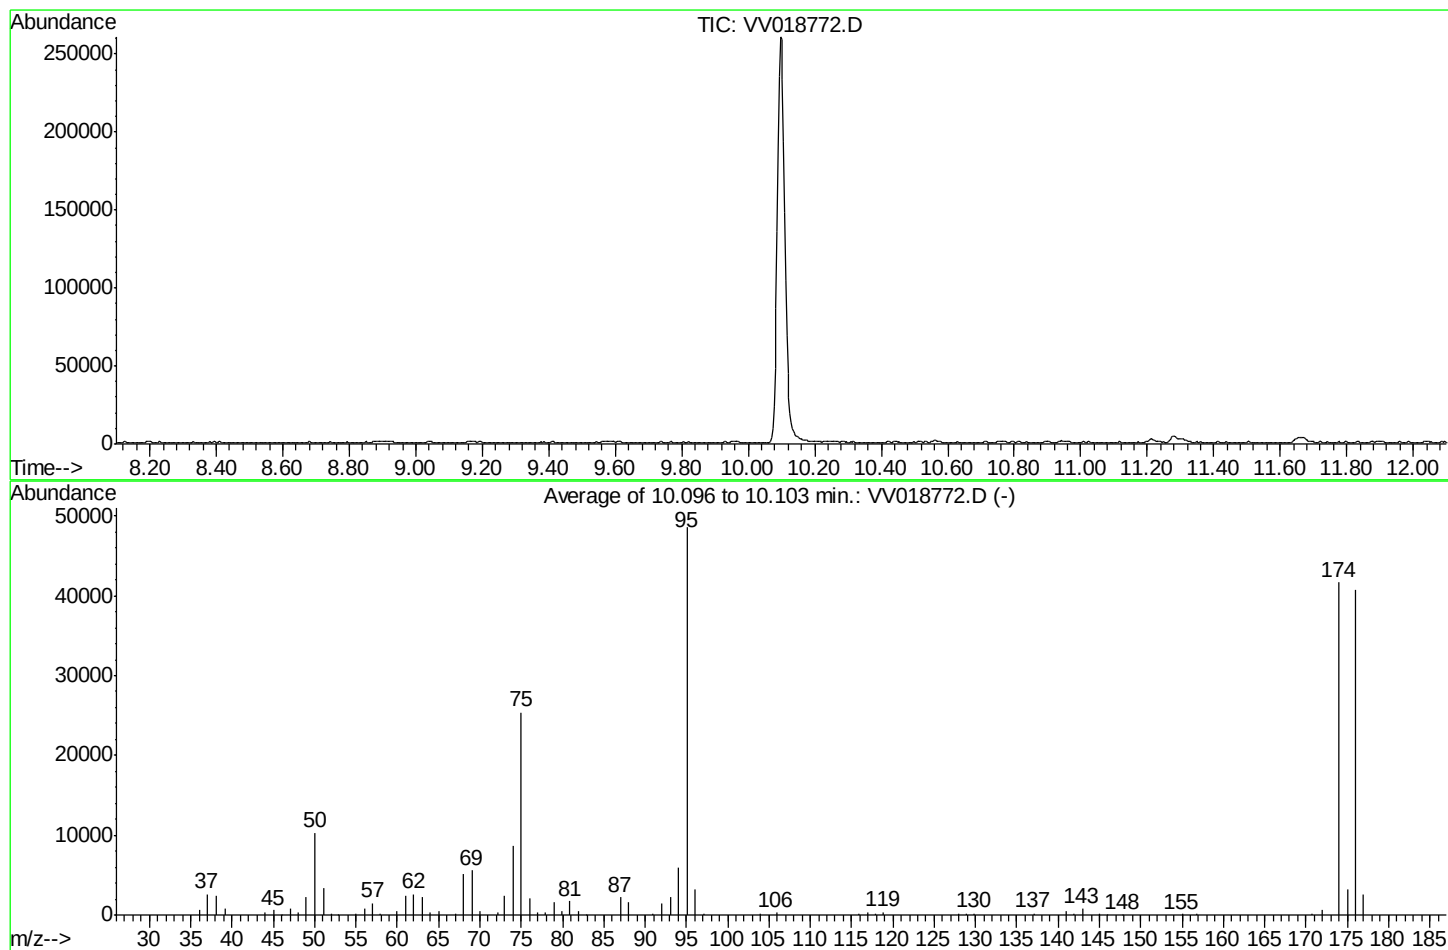

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	10333	PASS
75	95	30	80	52.3	25389	PASS
95	95	100	100	100.0	48576	PASS
96	95	5	9	6.7	3234	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.8	41666	PASS
175	174	5	9	7.6	3159	PASS
176	174	95	101	97.9	40776	PASS
177	176	5	9	6.2	2527	PASS

m/z	Abundance
36.00	687.0
37.00	2783.0
38.10	2458.0
39.10	911.0
40.00	252.0
44.00	981.0
45.00	667.0
46.00	122.0
47.00	741.0
48.00	436.0
49.00	2402.0
50.00	10997.0
51.10	3521.0
52.10	176.0
52.80	112.0
54.90	175.0
56.00	935.0
57.00	1654.0
57.90	123.0
59.90	557.0
61.00	2565.0
62.00	2814.0
63.00	2356.0
64.00	364.0
65.00	507.0
67.00	171.0
68.00	5311.0
69.00	5820.0
70.00	532.0
72.10	370.0
73.00	2604.0
74.10	9157.0
75.00	26944.0
76.00	2055.0
77.00	265.0
77.90	270.0
78.90	1710.0
79.90	563.0
80.90	1747.0
81.90	572.0
82.80	110.0
87.00	2269.0
88.00	1687.0
90.90	264.0
92.00	1520.0
93.10	2358.0
94.00	6323.0
95.00	50096.0
96.00	3534.0
97.10	160.0
103.90	255.0
105.90	282.0
115.90	241.0
116.90	345.0
117.90	132.0
118.80	388.0
128.00	258.0
129.80	226.0
137.10	133.0
140.90	583.0
141.80	160.0
143.00	773.0
144.90	202.0
145.90	128.0
147.80	106.0
155.00	112.0
156.90	113.0
170.80	139.0
171.90	614.0
174.00	42936.0
175.00	3250.0
176.00	41344.0
177.00	2537.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	640.0
37.00	2670.0
38.10	2546.0
39.10	912.0
40.00	242.0
44.00	987.0
45.00	619.0
47.00	811.0
48.00	383.0
49.00	2305.0
50.00	10697.0
51.10	3458.0
52.00	179.0
54.90	176.0
56.00	929.0
57.00	1589.0
57.90	134.0
60.00	450.0
61.00	2514.0
62.00	2708.0
63.00	2249.0
64.00	363.0
65.10	442.0
67.10	194.0
68.00	5258.0
69.00	5744.0
70.00	500.0
72.10	399.0
73.00	2479.0
74.10	9055.0
75.00	26104.0
76.00	2088.0
76.90	322.0
77.90	277.0
79.00	1630.0
79.90	539.0
80.90	1723.0
81.90	546.0
87.00	2302.0
88.00	1686.0
90.80	205.0
92.00	1529.0
93.10	2350.0
94.00	6197.0
95.10	50112.0
96.00	3324.0
97.10	125.0
103.90	232.0
106.00	280.0
115.90	198.0
117.00	363.0
117.90	146.0
118.90	411.0
127.90	204.0
128.90	146.0
129.90	216.0
137.00	189.0
140.90	542.0
141.90	164.0
143.00	766.0
145.00	199.0
145.90	103.0
147.80	120.0
155.00	136.0
156.80	124.0
170.80	136.0
171.90	688.0
174.00	43040.0
175.00	3255.0
176.00	42224.0
177.00	2599.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	564.0
37.00	2414.0
38.10	2381.0
39.10	830.0
39.90	240.0
44.00	950.0
45.00	496.0
47.00	775.0
47.90	289.0
49.00	2050.0
50.10	9306.0
51.00	3003.0
52.00	175.0
54.90	182.0
56.00	790.0
57.00	1318.0
57.90	105.0
60.10	392.0
61.00	2340.0
62.00	2378.0
63.00	2096.0
64.00	319.0
65.10	372.0
67.10	207.0
68.00	4864.0
69.00	5190.0
70.00	399.0
72.10	345.0
73.00	2223.0
74.00	7900.0
75.00	23120.0
76.00	1993.0
76.90	380.0
78.00	227.0
78.90	1444.0
79.90	440.0
80.90	1647.0
82.00	504.0
87.00	2005.0
88.00	1498.0
90.80	165.0
92.00	1439.0
93.00	2164.0
94.00	5472.0
95.10	45520.0
96.00	2846.0
103.90	219.0
106.00	260.0
115.80	168.0
117.00	360.0
117.90	162.0
118.90	370.0
127.80	154.0
128.80	198.0
129.90	194.0
137.00	177.0
140.90	525.0
141.90	176.0
142.90	707.0
144.90	146.0
155.00	157.0
156.80	137.0
170.80	116.0
171.90	677.0
174.00	39024.0
175.00	2974.0
176.00	38760.0
177.00	2445.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

Scan 2790 (10.061 min): VV018772.D
BFB70

m/z	Abundance
39.90	246.0
44.00	714.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70