

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032349.D
 Acq On : 09 Oct 2023 23:51
 Operator : SY/MD
 Sample : 04774-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 10 06:01:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 10 05:42:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	108711	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	119778	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	55233	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	41904	4.740	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.800%
7) Chloroethane-d5	1.532	69	33387	4.652	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.060	65	15825	4.244	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.800%
20) 2-Butanone-d5	3.815	46	95683	42.781	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.560%
24) Chloroform-d	4.253	84	65102	4.174	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.400%
26) 1,2-Dichloroethane-d4	4.950	65	31747	4.297	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
32) Benzene-d6	4.963	84	126612	3.592	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.800%
36) 1,2-Dichloropropane-d6	5.995	67	42047	3.601	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.000%
41) Toluene-d8	7.246	98	122686	3.807	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	7.561	79	13895	3.358	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.200%
46) 2-Hexanone-d5	8.031	63	73202	37.599	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.200%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	32476	3.976	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	44578	4.349	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.000%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.188	75	7163	1.218	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032349.D
Acq On : 09 Oct 2023 23:51
Operator : SY/MD
Sample : 04774-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 10 06:01:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 10 05:42:01 2023
Response via : Initial Calibration

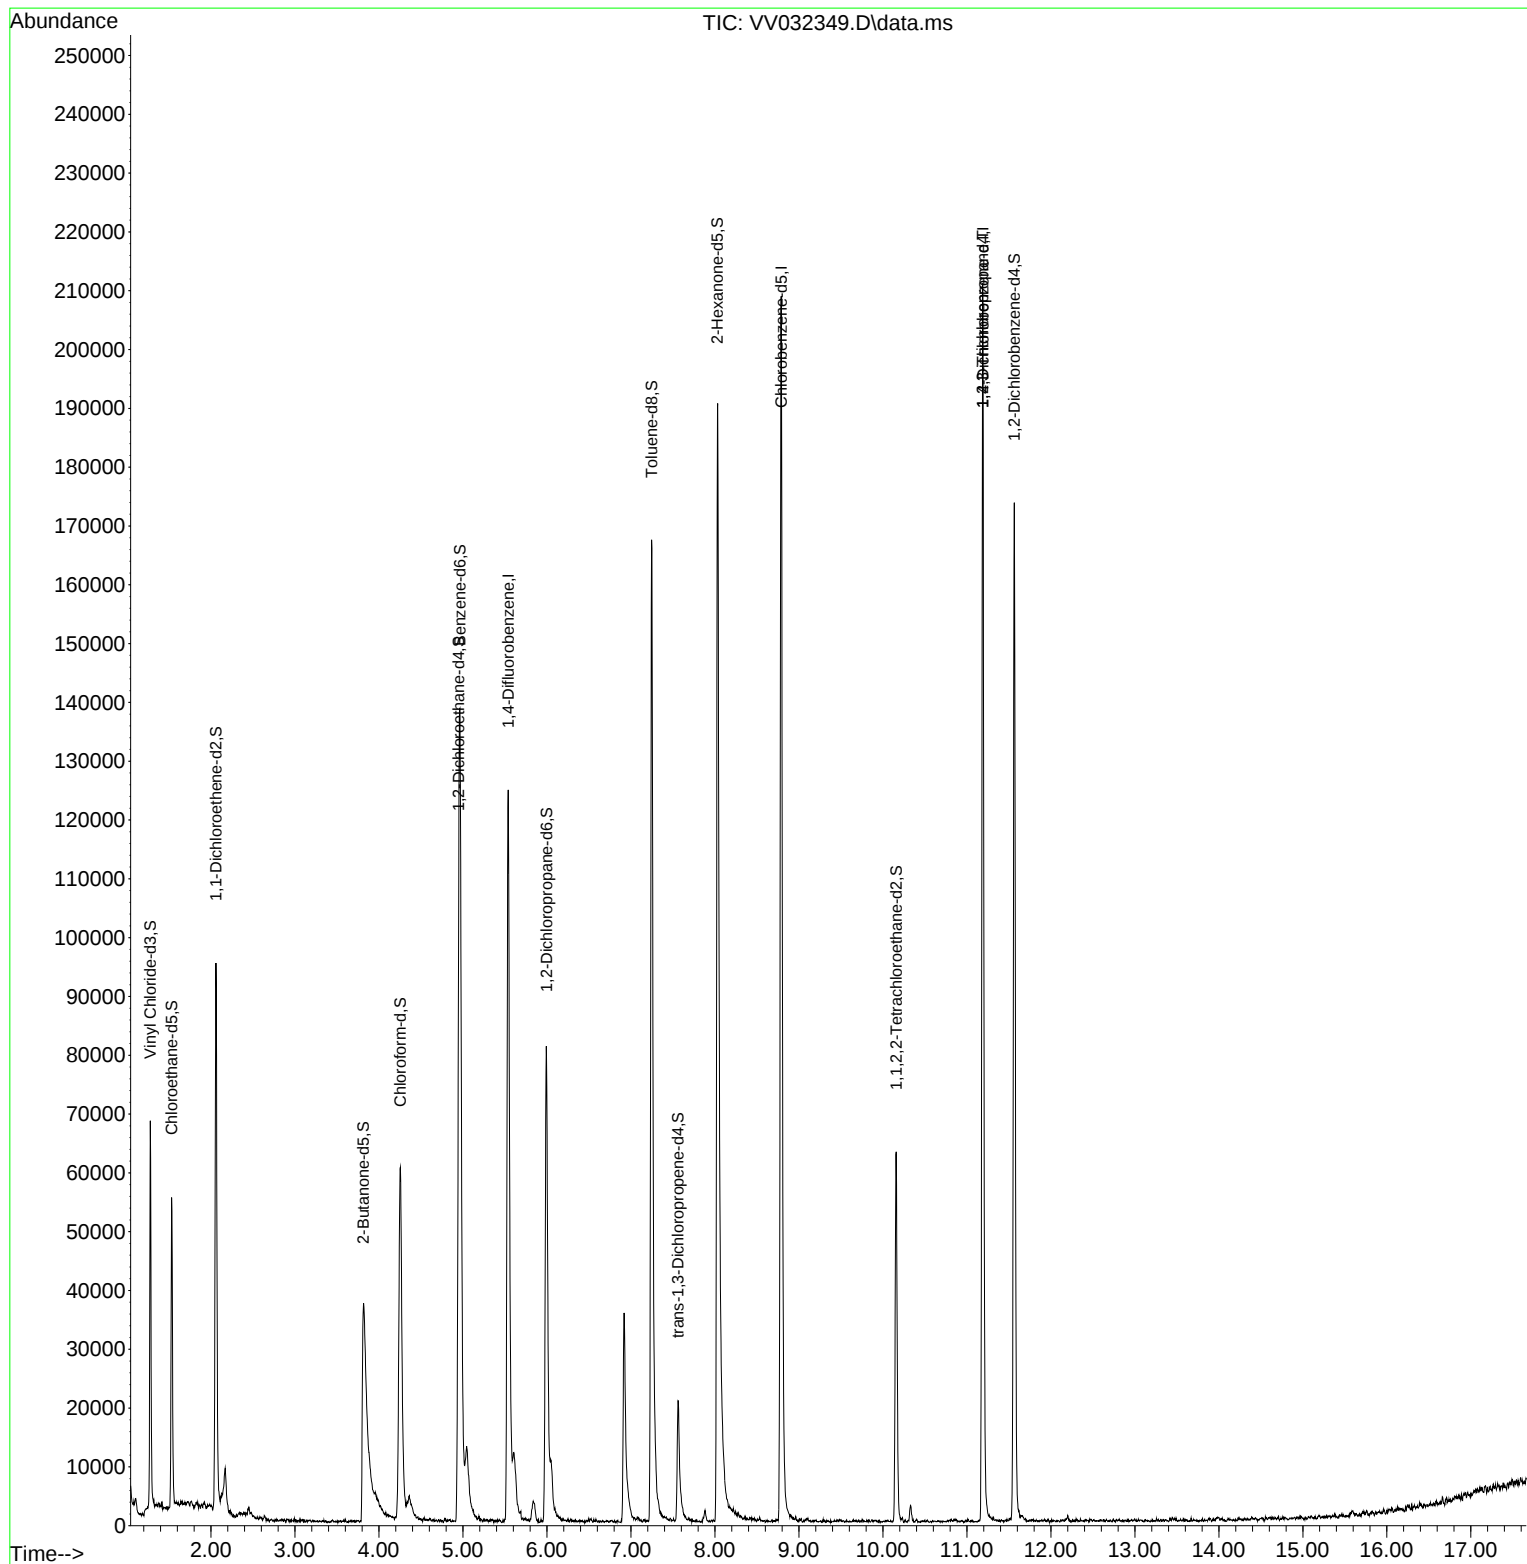

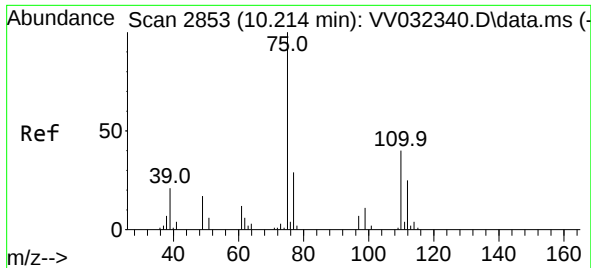

#61

1,2,3-Trichloropropane

Concen: 1.218 ug/L

RT: 11.188 min Scan# 31

Delta R.T. 0.974 min


Lab File: VV032349.D

Acq: 09 Oct 2023 23:51

Instrument :

MSVOA_V

ClientSampleId :

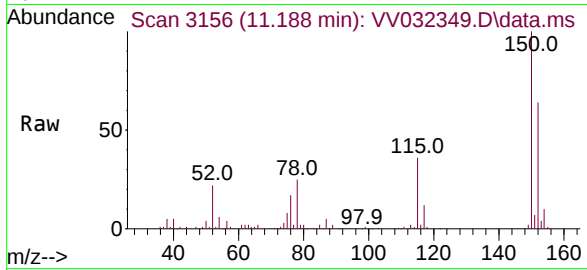

Tgt Ion: 75 Resp: 7163

Ion Ratio Lower Upper

75 100

77 30.6 26.2 39.2

110 1.5 30.6 46.0#

