

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032328.D
 Acq On : 09 Oct 2023 14:58
 Operator : SY/MD
 Sample : 04741-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B01

Quant Time: Oct 10 04:51:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 07 05:00:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	102148	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	110771	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	50973	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	46578	5.607	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.200%
7) Chloroethane-d5	1.532	69	36365	5.393	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.800%
11) 1,1-Dichloroethene-d2	2.060	65	17649	5.037	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.800%
20) 2-Butanone-d5	3.815	46	98846	47.035	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.060%
24) Chloroform-d	4.252	84	73512	5.016	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	4.947	65	34399	4.955	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	4.963	84	143316	4.397	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	5.995	67	44454	4.116	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.400%
41) Toluene-d8	7.249	98	135944	4.561	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	7.561	79	15108	3.948	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.000%
46) 2-Hexanone-d5	8.030	63	75233	41.784	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.560%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	33566	4.444	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.800%
66) 1,2-Dichlorobenzene-d4	11.564	152	48456	5.123	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds						
25) Chloroform	4.281	83	29756	1.879	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032328.D
Acq On : 09 Oct 2023 14:58
Operator : SY/MD
Sample : 04741-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B01

Quant Time: Oct 10 04:51:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 07 05:00:49 2023
Response via : Initial Calibration

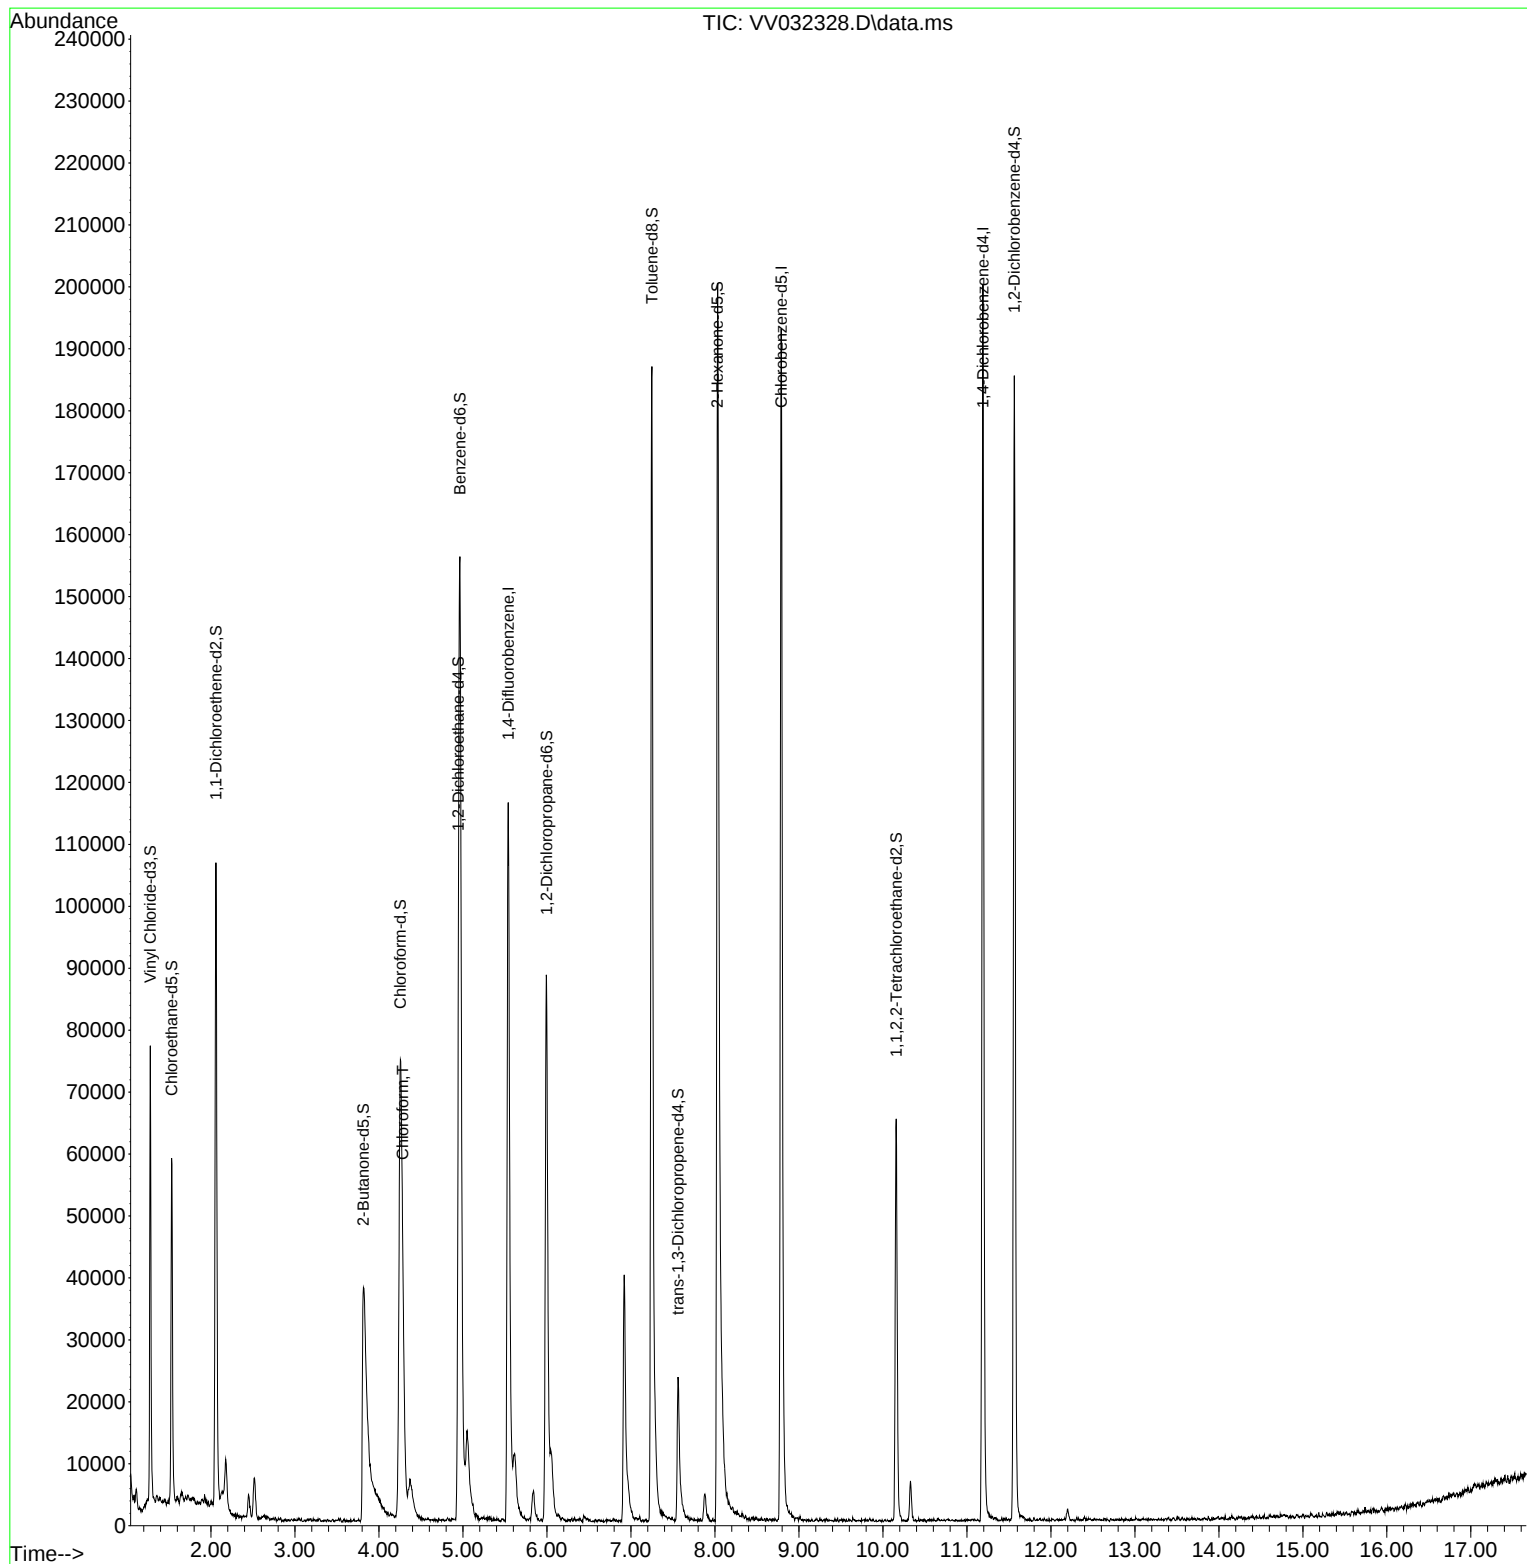

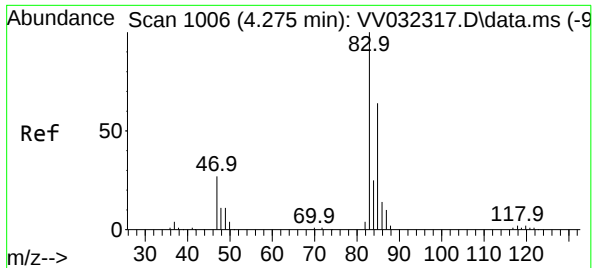

#25
 Chloroform
 Concen: 1.879 ug/L
 RT: 4.281 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV032328.D
 Acq: 09 Oct 2023 14:58

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B01

Tgt Ion: 83 Resp: 29756
 Ion Ratio Lower Upper
 83 100
 85 64.2 45.4 84.4

