

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100923\
 Data File : VW032342.D
 Acq On : 09 Oct 2023 21:00
 Operator : SY/MD
 Sample : 04748-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX885

Quant Time: Oct 10 05:59:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 10 05:42:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	101111	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	107921	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	47610	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	40965	4.982	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.600%
7) Chloroethane-d5	1.532	69	32142	4.815	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.400%
11) 1,1-Dichloroethene-d2	2.060	65	14824	4.274	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.400%
20) 2-Butanone-d5	3.809	46	89050	42.808	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.620%
24) Chloroform-d	4.253	84	64174	4.424	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	4.947	65	31418	4.572	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	4.963	84	122991	3.873	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.400%
36) 1,2-Dichloropropane-d6	5.992	67	40199	3.821	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.400%
41) Toluene-d8	7.246	98	114145	3.931	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.600%
43) trans-1,3-Dichloroprop...	7.561	79	13916	3.733	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.600%
46) 2-Hexanone-d5	8.031	63	78945	45.004	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.000%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	33414	4.541	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	11.564	152	40320	4.564	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds						Qvalue
13) Acetone	2.137	43	2802	1.748	ug/L	77
18) trans-1,2-Dichloroethene	2.696	96	14210	1.673	ug/L	96
22) cis-1,2-Dichloroethene	3.822	96	12908	1.411	ug/L	97
25) Chloroform	4.285	83	25443	1.623	ug/L	97
30) Cyclohexane	4.587	56	2470	0.153	ug/L	97
31) Carbon tetrachloride	4.738	117	177760	14.318	ug/L	99
34) Trichloroethene	5.838	95	54373	5.242	ug/L	98
35) Methylcyclohexane	6.053	83	5436	0.339	ug/L #	81
42) Toluene	7.326	91	13833	0.342	ug/L	98
52) Ethylbenzene	8.957	91	4858	0.108	ug/L	94
53) m,p-Xylene	9.085	106	3272	0.196	ug/L	92
54) o-Xylene	9.490	106	1270	0.079	ug/L	96
63) 1,2,4-Trimethylbenzene	10.860	105	3589	0.120	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032342.D
Acq On : 09 Oct 2023 21:00
Operator : SY/MD
Sample : 04748-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX885

Quant Time: Oct 10 05:59:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 10 05:42:01 2023
Response via : Initial Calibration

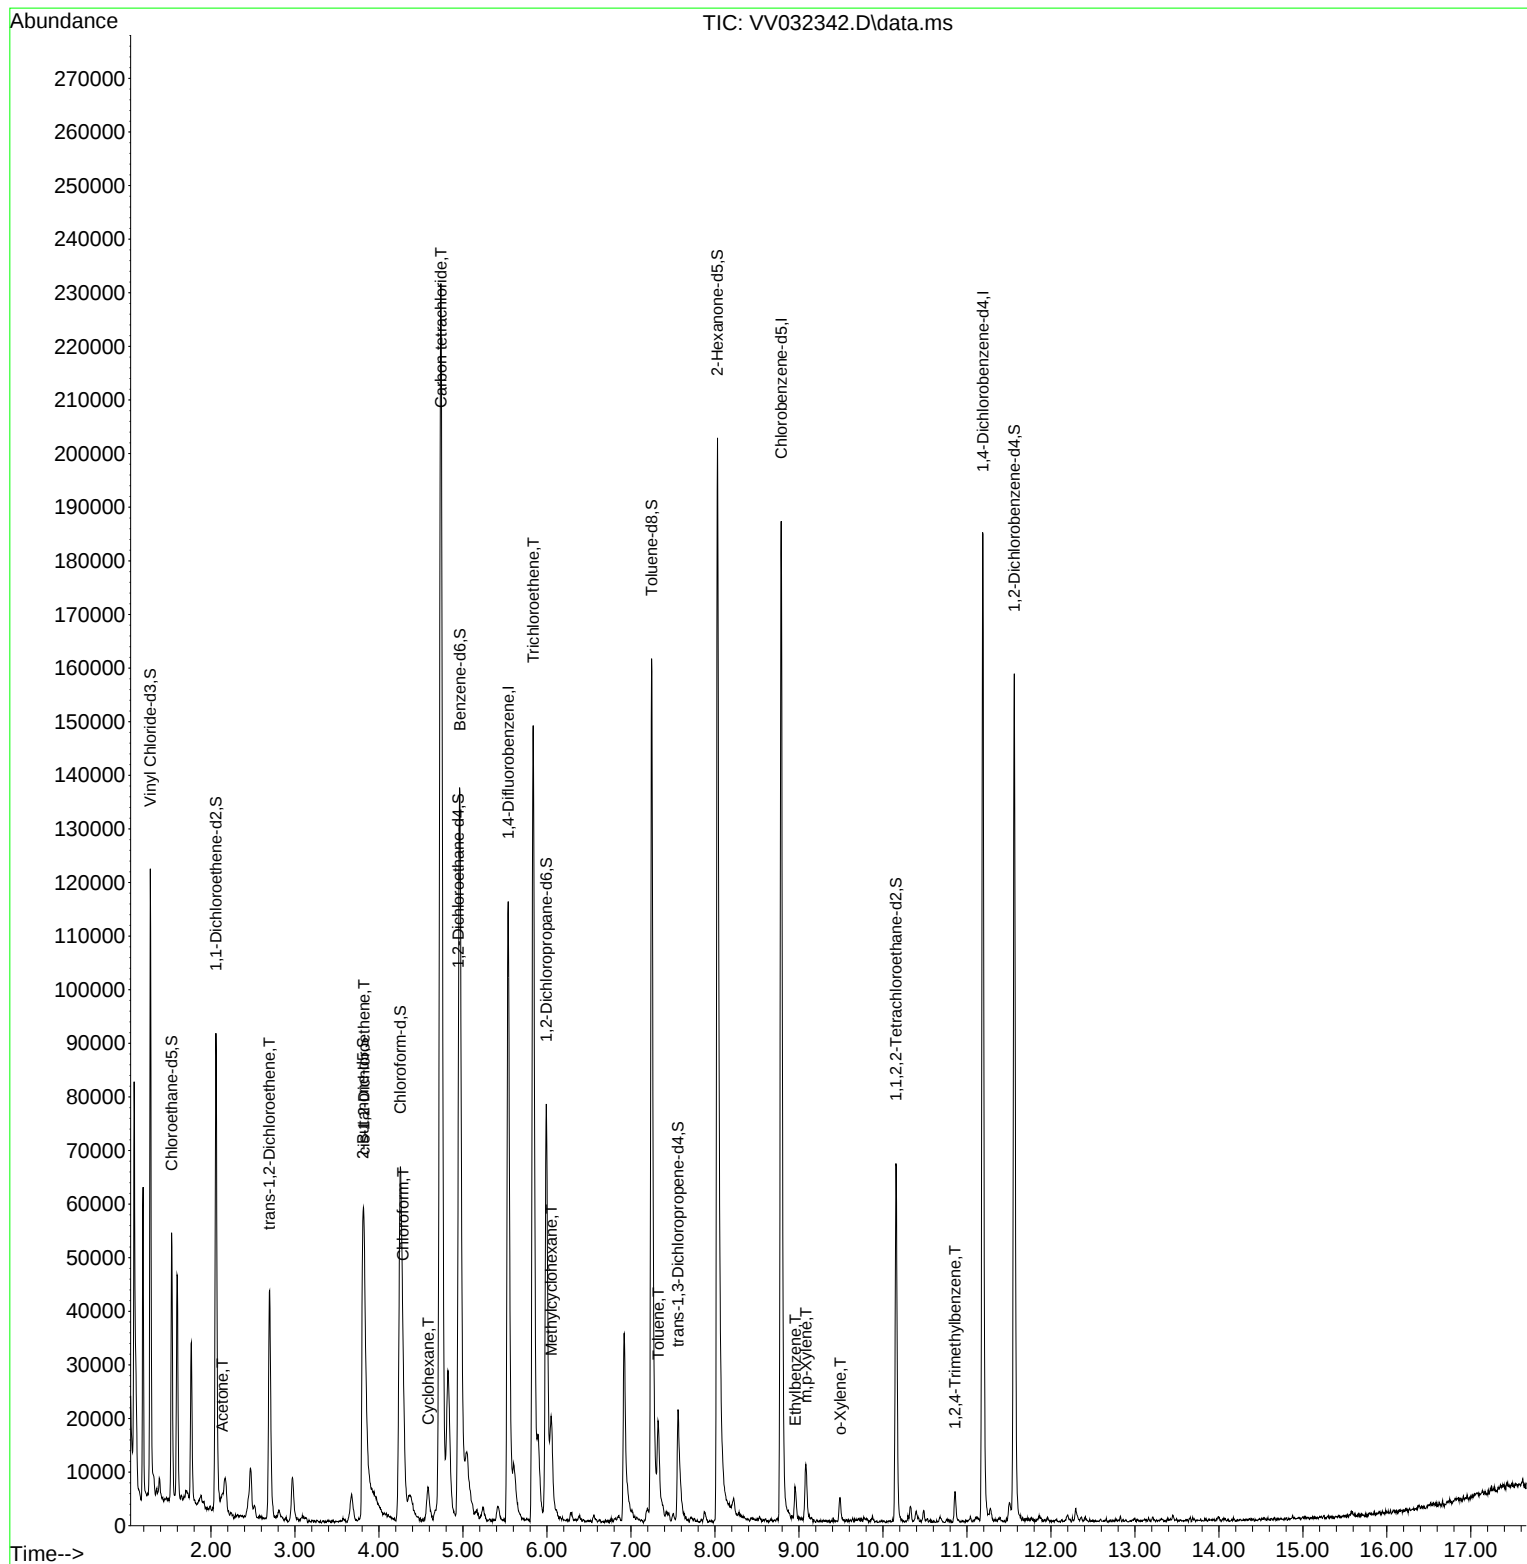

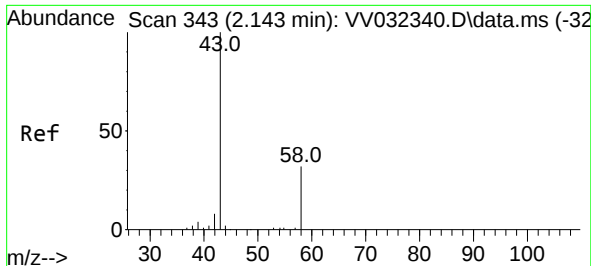

#13

Acetone

Concen: 1.748 ug/L

RT: 2.137 min Scan# 34

Delta R.T. -0.006 min

Lab File: VV032342.D

Acq: 09 Oct 2023 21:00

Instrument :

MSVOA_V

ClientSampleId :





EX885

Tgt Ion: 43 Resp: 2802

Ion Ratio Lower Upper

43 100

58 45.8 0.0 66.0

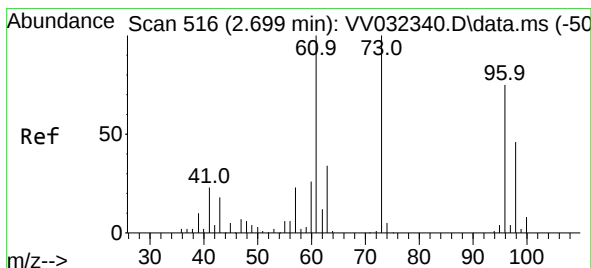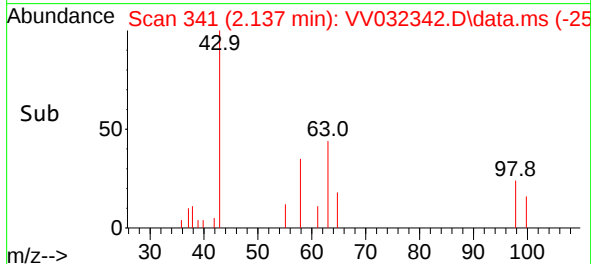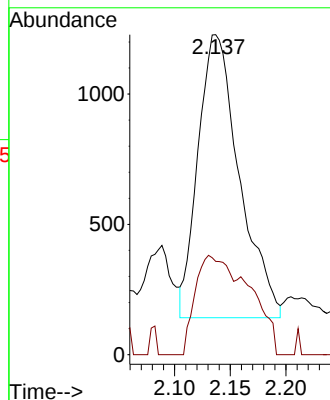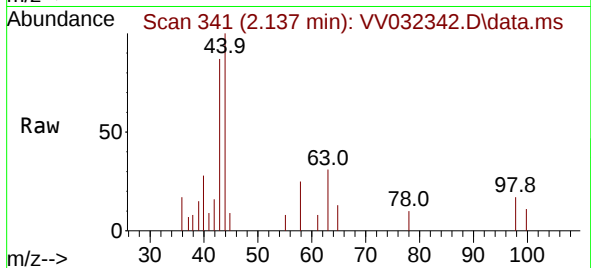

#18

trans-1,2-Dichloroethene

Concen: 1.673 ug/L

RT: 2.696 min Scan# 515

Delta R.T. -0.003 min

Lab File: VV032342.D

Acq: 09 Oct 2023 21:00




Tgt Ion: 96 Resp: 14210


Ion Ratio Lower Upper

96 100

61 143.2 96.9 180.1

98 62.4 45.3 84.1


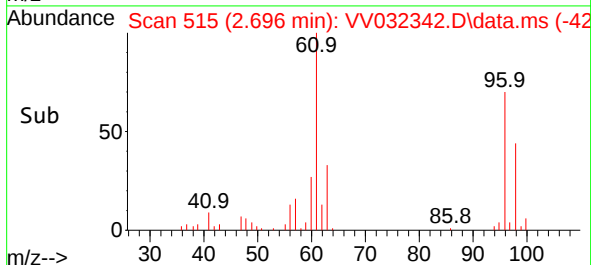
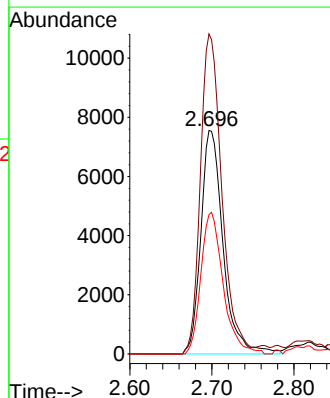
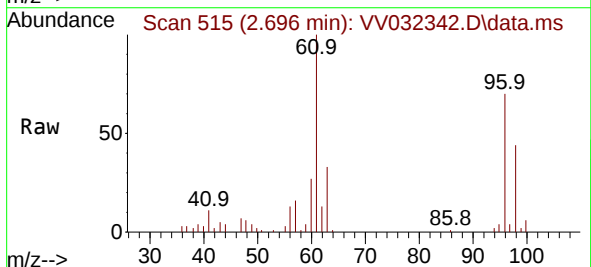


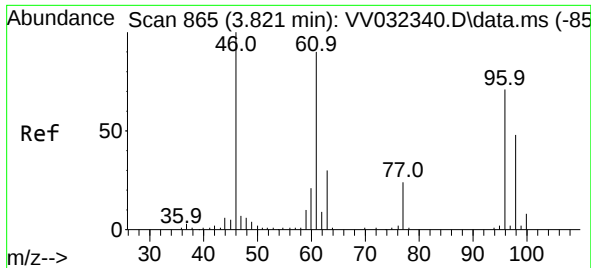

#22
cis-1,2-Dichloroethene
Concen: 1.411 ug/L
RT: 3.822 min Scan# 80
Delta R.T. 0.000 min
Lab File: VV032342.D
Acq: 09 Oct 2023 21:00




Instrument :
MSVOA_V
ClientSampleId :
EX885


Tgt Ion: 96 Resp: 12908
Ion Ratio Lower Upper
96 100
61 126.2 85.8 159.4
98 61.5 44.0 81.6

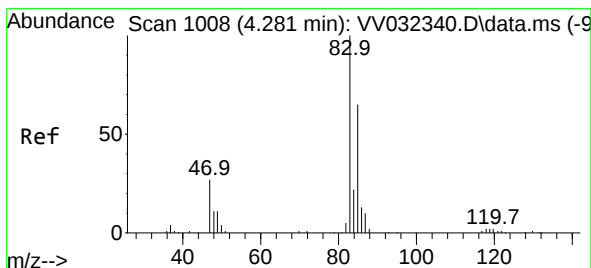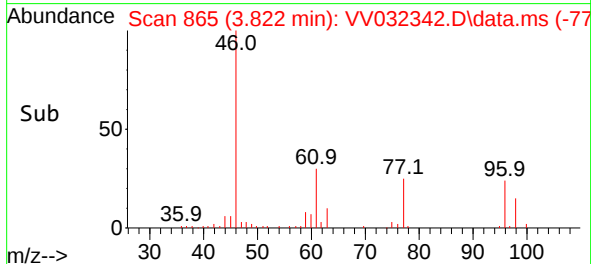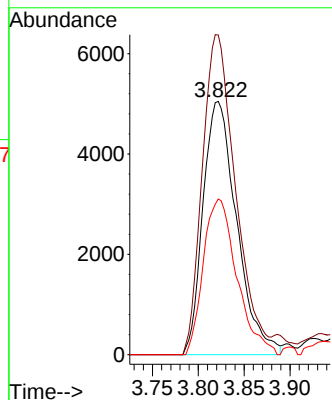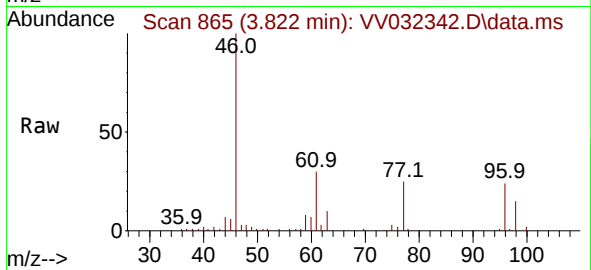

#25
Chloroform
Concen: 1.623 ug/L
RT: 4.285 min Scan# 1009
Delta R.T. 0.003 min
Lab File: VV032342.D
Acq: 09 Oct 2023 21:00

Tgt Ion: 83 Resp: 25443
Ion Ratio Lower Upper
83 100
85 67.6 45.4 84.4

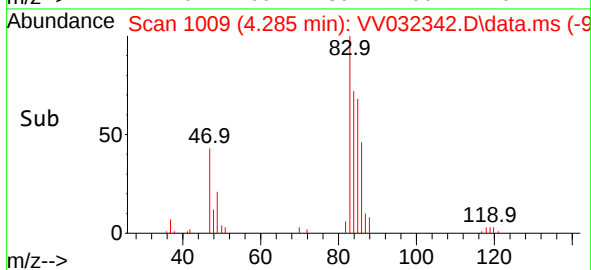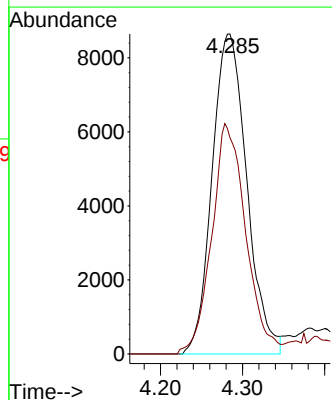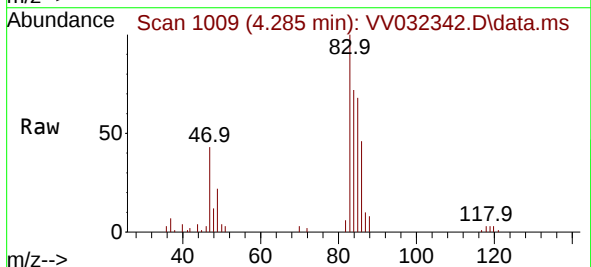

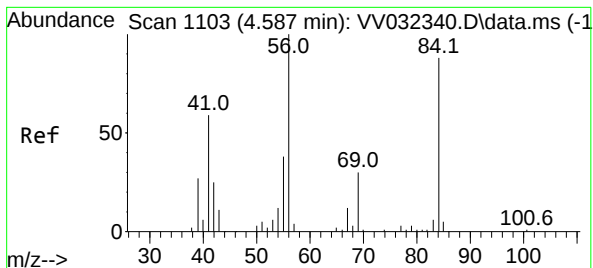

#30

Cyclohexane

Concen: 0.153 ug/L

RT: 4.587 min Scan# 1103

Delta R.T. 0.000 min

Lab File: VV032342.D

Acq: 09 Oct 2023 21:00

Instrument :

MSVOA_V

ClientSampleId :

EX885





Tgt Ion: 56 Resp: 2470

Ion Ratio Lower Upper

56 100

69 26.3 24.2 36.2

84 86.6 68.1 102.1

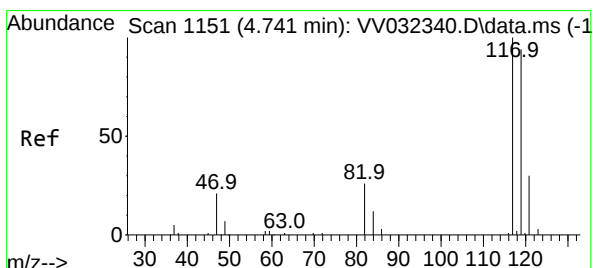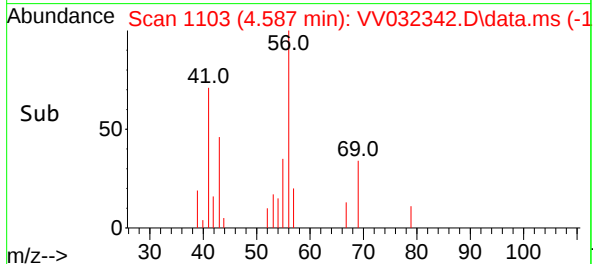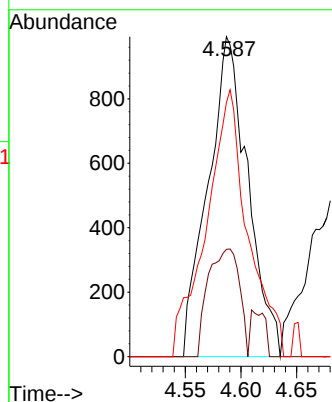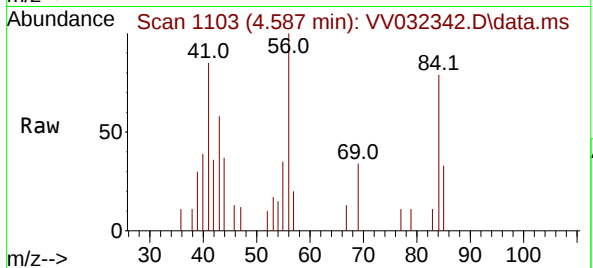

#31

Carbon tetrachloride

Concen: 14.318 ug/L

RT: 4.738 min Scan# 1150

Delta R.T. -0.003 min

Lab File: VV032342.D




Acq: 09 Oct 2023 21:00


Tgt Ion: 117 Resp: 177760

Ion Ratio Lower Upper

117 100

119 95.8 77.6 116.4

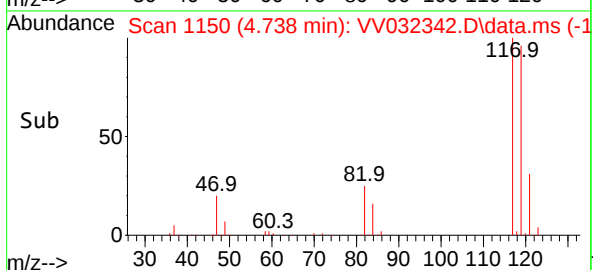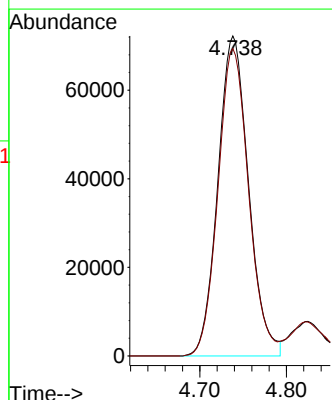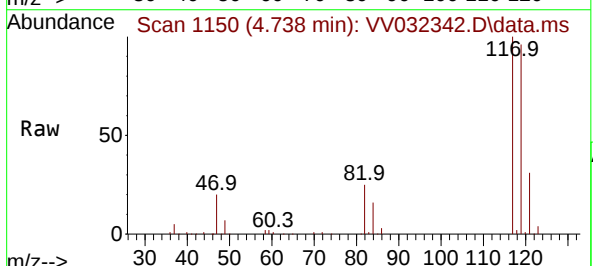




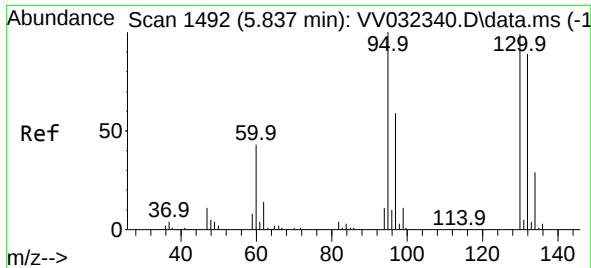


#34
Trichloroethene
Concen: 5.242 ug/L
RT: 5.838 min Scan# 1492
Delta R.T. 0.000 min
Lab File: VV032342.D
Acq: 09 Oct 2023 21:00

Instrument :
MSVOA_V
ClientSampleId :
EX885

Tgt Ion: 95 Resp: 54373




Ion	Ratio	Lower	Upper
95	100		
97	62.7	45.7	84.9
132	96.7	70.3	130.5
130	99.3	69.6	129.2

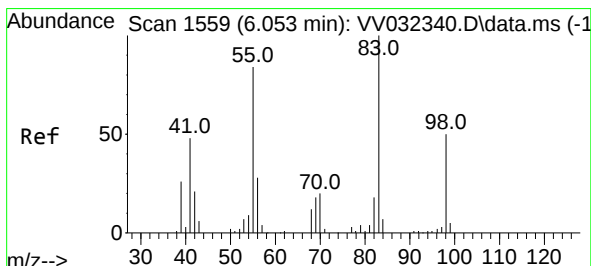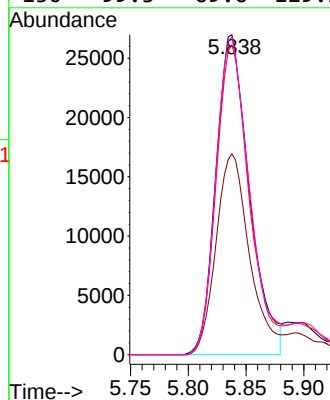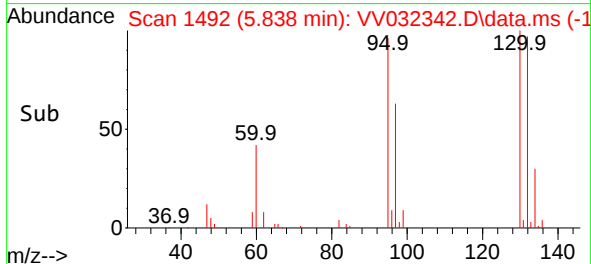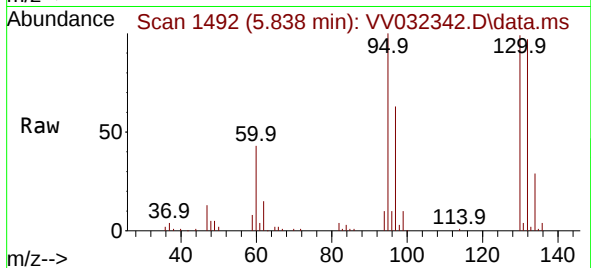


#35
Methylcyclohexane
Concen: 0.339 ug/L
RT: 6.053 min Scan# 1559
Delta R.T. 0.000 min
Lab File: VV032342.D
Acq: 09 Oct 2023 21:00

Tgt Ion: 83 Resp: 5436

Ion	Ratio	Lower	Upper
83	100		
55	67.0	64.2	96.2
98	32.2	39.6	59.4

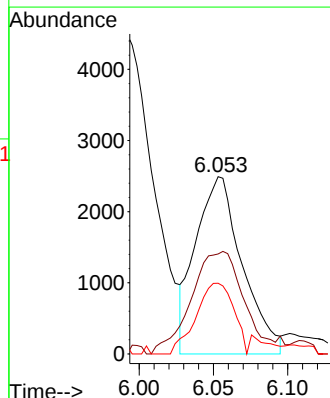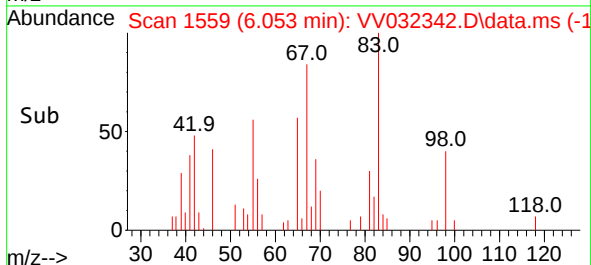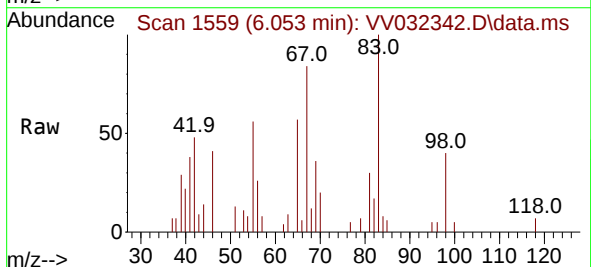

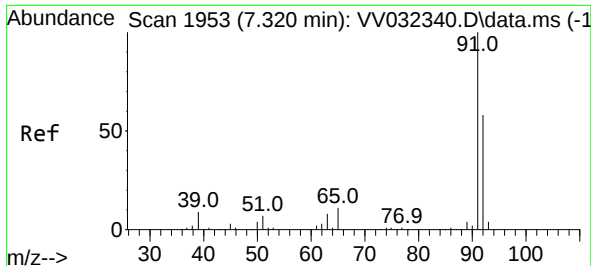

#42

Toluene

Concen: 0.342 ug/L

RT: 7.326 min Scan# 1953

Delta R.T. 0.007 min

Lab File: VV032342.D

Acq: 09 Oct 2023 21:00

Instrument :

MSVOA_V

ClientSampleId :





EX885

Tgt Ion: 91 Resp: 13833

Ion Ratio Lower Upper

91 100

92 56.8 40.8 75.8

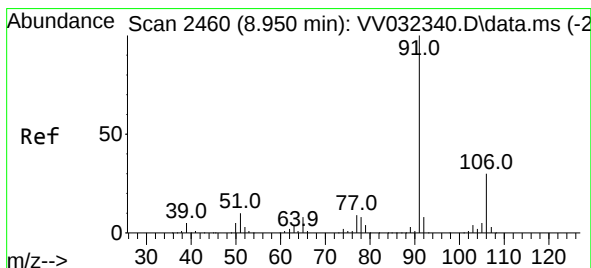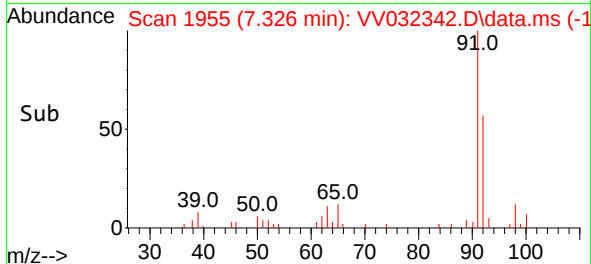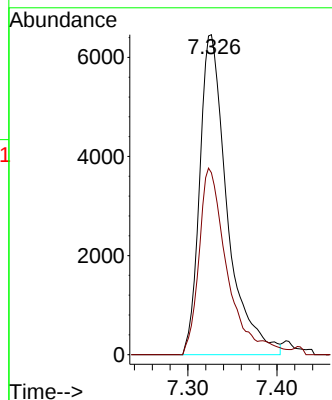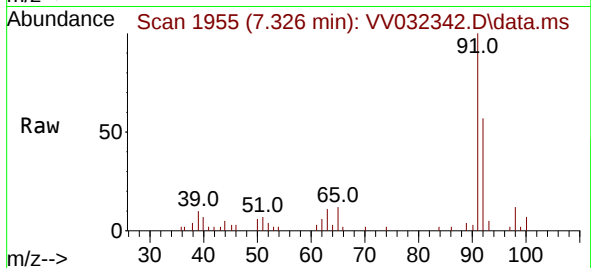

#52

Ethylbenzene

Concen: 0.108 ug/L

RT: 8.957 min Scan# 2462

Delta R.T. 0.007 min

Lab File: VV032342.D




Acq: 09 Oct 2023 21:00


Tgt Ion: 91 Resp: 4858

Ion Ratio Lower Upper

91 100

106 27.3 21.3 39.5

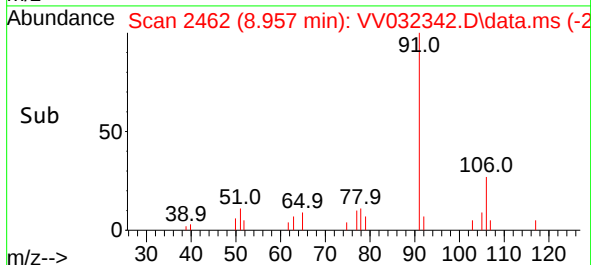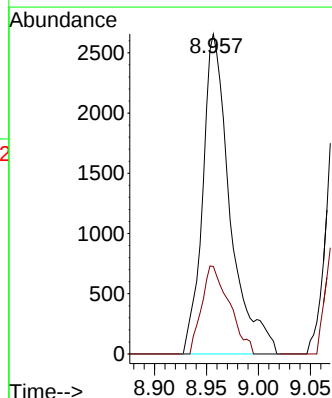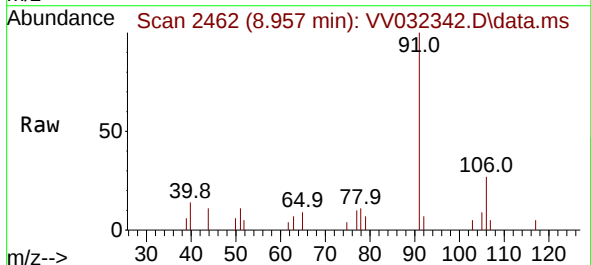

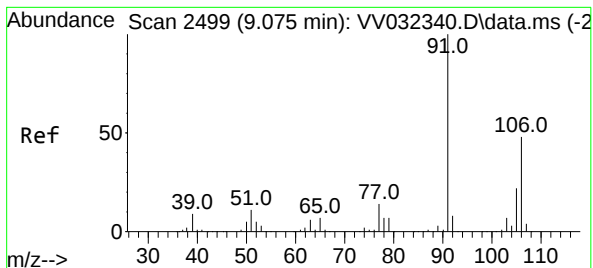

#53

m,p-Xylene

Concen: 0.196 ug/L

RT: 9.085 min Scan# 21

Delta R.T. 0.010 min

Lab File: VV032342.D

Acq: 09 Oct 2023 21:00

Instrument :

MSVOA_V

ClientSampleId :





EX885

Tgt Ion:106 Resp: 3272

Ion Ratio Lower Upper

106 100

91 194.4 144.5 268.3

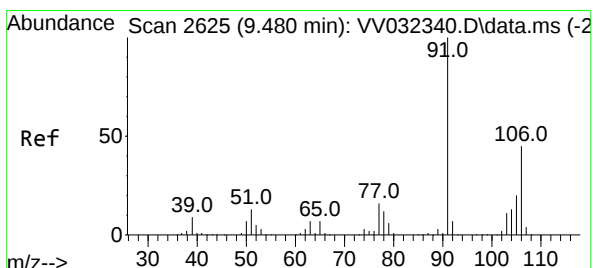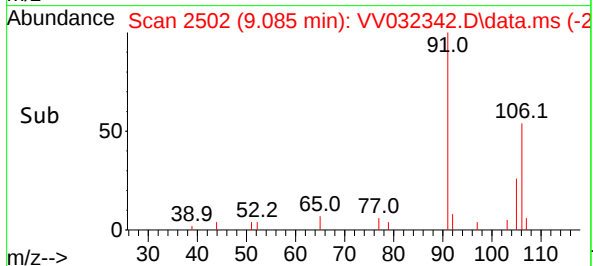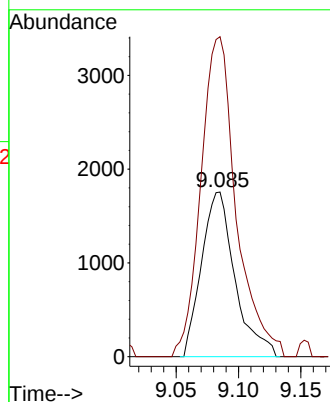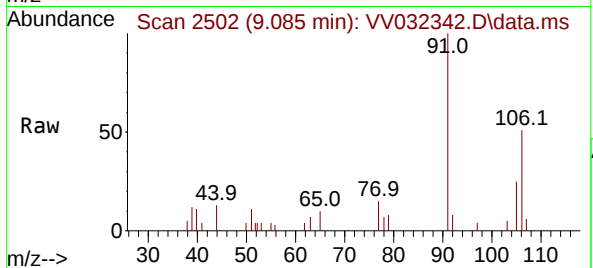

#54

o-Xylene

Concen: 0.079 ug/L

RT: 9.490 min Scan# 2628

Delta R.T. 0.010 min

Lab File: VV032342.D




Acq: 09 Oct 2023 21:00


Tgt Ion:106 Resp: 1270

Ion Ratio Lower Upper

106 100

91 215.4 154.8 287.4

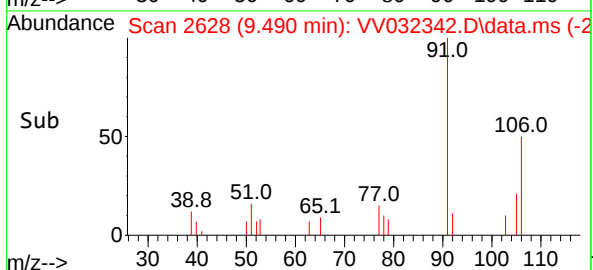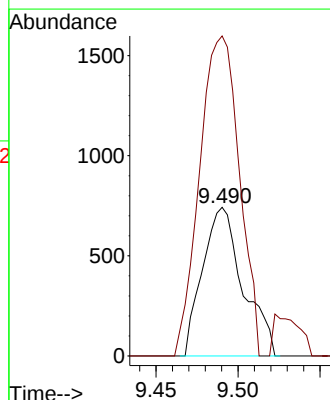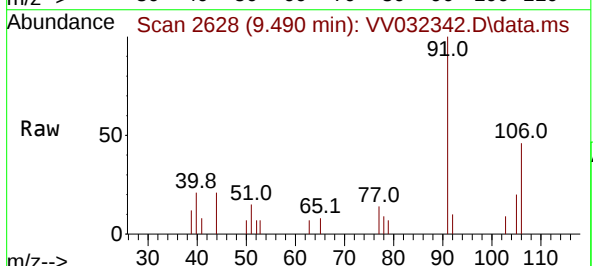

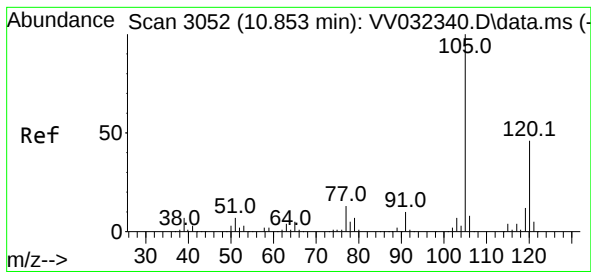

#63

1,2,4-Trimethylbenzene

Concen: 0.120 ug/L

RT: 10.860 min Scan# 30

Delta R.T. 0.007 min

Lab File: VV032342.D


Acq: 09 Oct 2023 21:00

Instrument :

MSVOA_V

ClientSampleId :

EX885

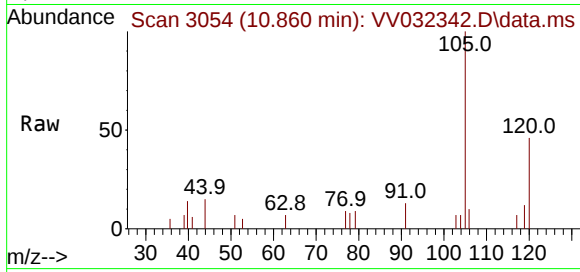

Tgt Ion:105 Resp: 3589

Ion Ratio Lower Upper

105 100

120 45.8 36.2 54.4

