

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032320.D
 Acq On : 09 Oct 2023 11:45
 Operator : SY/MD
 Sample : 04708-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJS6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	78382	78213	17.20%	2.151%
2	1.532	146	153	168	rVB	61569	72210	15.88%	1.986%
3	2.060	308	317	330	rBV	107479	156269	34.36%	4.298%
4	3.806	852	860	893	rBV	45694	146427	32.20%	4.027%
5	4.256	986	1000	1019	rBV	68376	179445	39.46%	4.935%
6	4.960	1205	1219	1238	rBV3	162335	412179	90.63%	11.335%
7	5.539	1388	1399	1416	rBV	119021	250932	55.18%	6.901%
8	5.838	1482	1492	1500	rBV7	3836	7779	1.71%	0.214%
9	5.992	1528	1540	1573	rBV2	90686	212928	46.82%	5.856%
10	6.918	1818	1828	1860	rBV3	41028	94977	20.88%	2.612%
11	7.249	1919	1931	1967	rBV	196632	379857	83.52%	10.446%
12	7.561	2019	2028	2055	rBV3	24077	51693	11.37%	1.422%
13	7.883	2115	2128	2143	rBV2	7837	15315	3.37%	0.421%
14	8.030	2164	2174	2208	rBV	209078	454787	100.00%	12.507%
15	8.789	2399	2410	2434	rBV	195008	336938	74.09%	9.266%
16	9.014	2471	2480	2486	rBV4	3275	5329	1.17%	0.147%
17	10.159	2825	2836	2853	rBV	68788	113463	24.95%	3.120%
18	10.329	2879	2889	2902	rVB2	17923	29604	6.51%	0.814%
19	11.188	3146	3156	3176	rBV	197957	314757	69.21%	8.656%
20	11.564	3263	3273	3299	rVB	195600	311753	68.55%	8.573%
21	12.201	3460	3471	3479	rVB	6972	11391	2.50%	0.313%




Sum of corrected areas: 3636246

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032320.D
Acq On : 09 Oct 2023 11:45
Operator : SY/MD
Sample : 04708-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

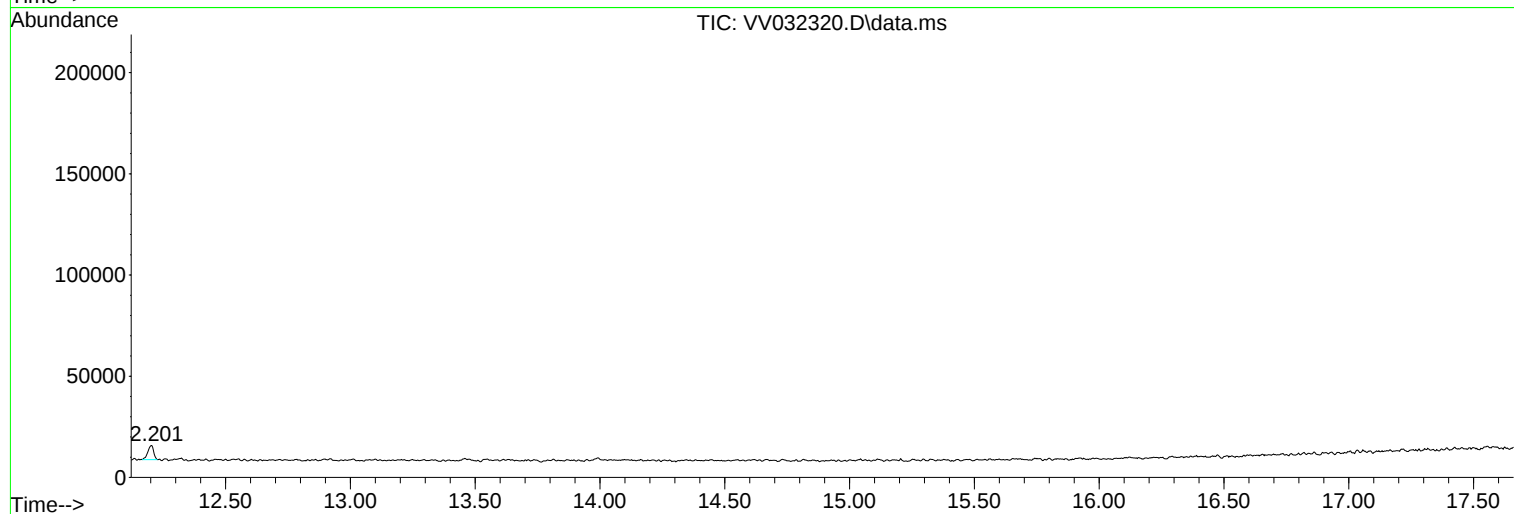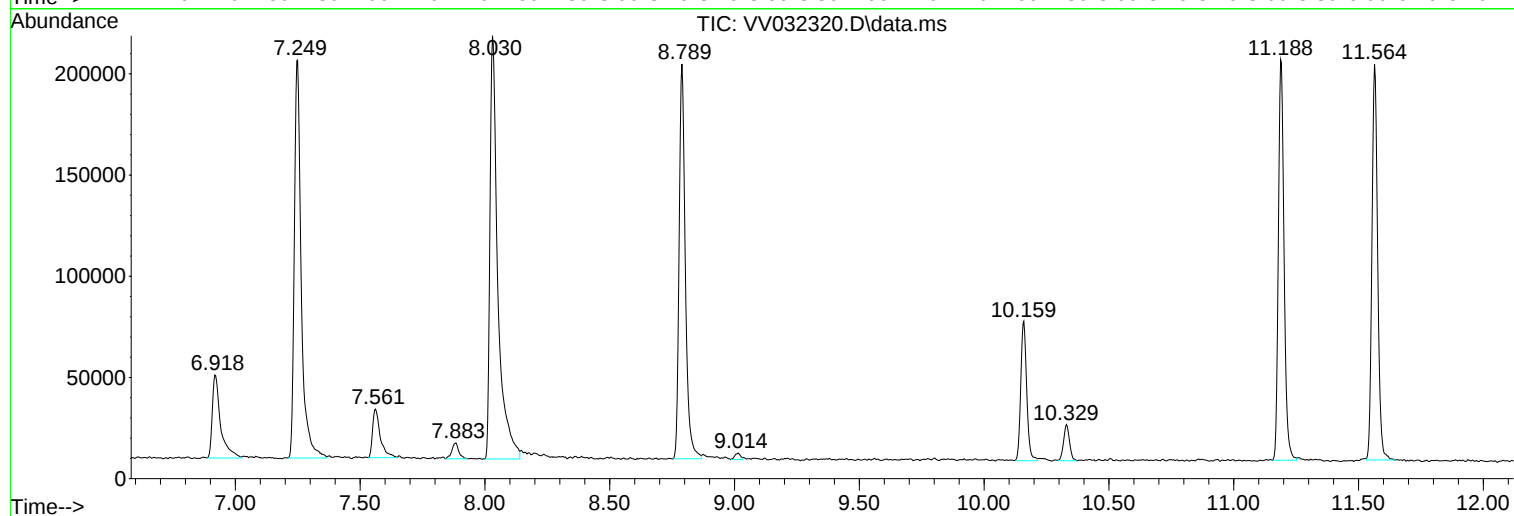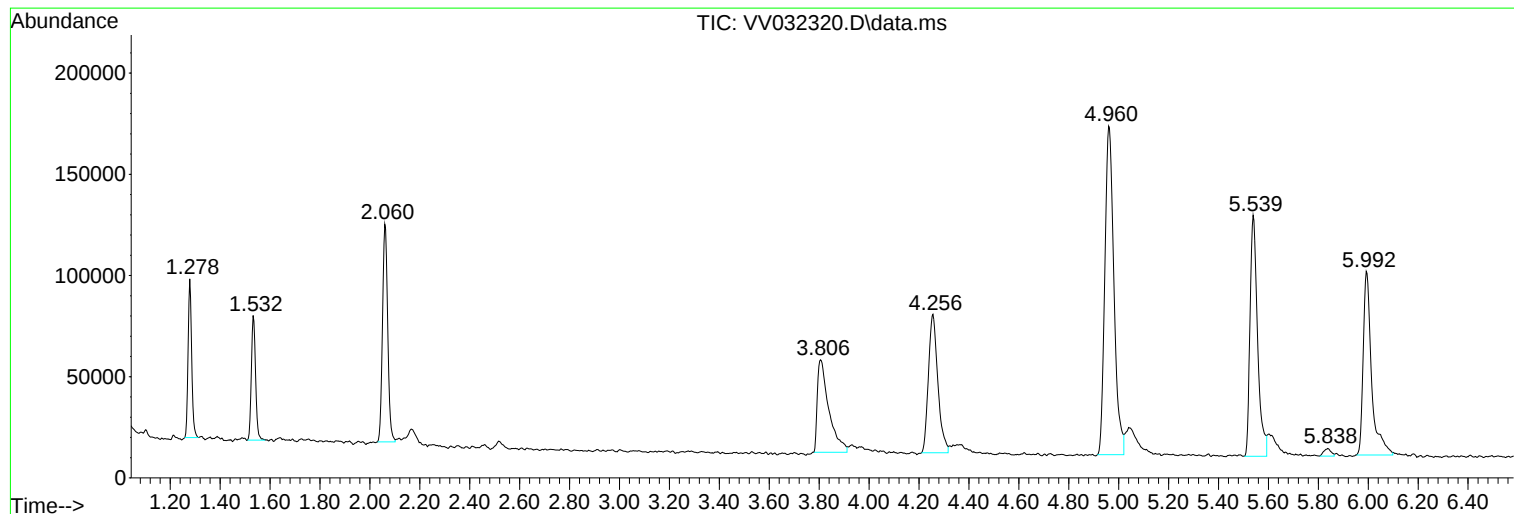

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032320.D
Acq On : 09 Oct 2023 11:45
Operator : SY/MD
Sample : 04708-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032320.D
Acq On : 09 Oct 2023 11:45
Operator : SY/MD
Sample : 04708-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc