

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
 Data File : VV032321.D
 Acq On : 09 Oct 2023 12:09
 Operator : SY/MD
 Sample : 04708-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJS9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	75581	81297	18.13%	2.234%
2	1.532	145	153	163	rBV	59689	70720	15.77%	1.944%
3	2.060	307	317	331	rBV	107707	158213	35.28%	4.348%
4	2.162	346	349	362	rVB4	8161	15119	3.37%	0.416%
5	2.304	380	393	396	rBV8	6566	13009	2.90%	0.358%
6	3.809	852	861	892	rBV2	47727	159828	35.64%	4.393%
7	4.252	983	999	1019	rBV	67292	181313	40.43%	4.983%
8	4.960	1203	1219	1238	rBV3	162091	414193	92.35%	11.383%
9	5.538	1388	1399	1415	rBV	117790	245547	54.75%	6.748%
10	5.838	1481	1492	1508	rVB8	4303	8755	1.95%	0.241%
11	5.992	1528	1540	1555	rBV2	90939	196346	43.78%	5.396%
12	6.921	1817	1829	1859	rBV	41081	90859	20.26%	2.497%
13	7.246	1918	1930	1961	rBV	192919	377849	84.25%	10.384%
14	7.561	2019	2028	2045	rBV	25060	49061	10.94%	1.348%
15	7.882	2116	2128	2138	rBV3	7601	14784	3.30%	0.406%
16	8.030	2165	2174	2205	rBV	208096	448503	100.00%	12.326%
17	8.789	2399	2410	2435	rBV	196622	341751	76.20%	9.392%
18	10.159	2825	2836	2852	rBV	66975	110667	24.67%	3.041%
19	10.329	2878	2889	2902	rVB3	14495	23531	5.25%	0.647%
20	11.191	3146	3157	3176	rBV	203768	317742	70.85%	8.732%
21	11.564	3261	3273	3294	rBV	194046	310789	69.29%	8.541%
22	12.197	3463	3470	3482	rVB2	5427	8756	1.95%	0.241%




Sum of corrected areas: 3638632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032321.D
Acq On : 09 Oct 2023 12:09
Operator : SY/MD
Sample : 04708-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

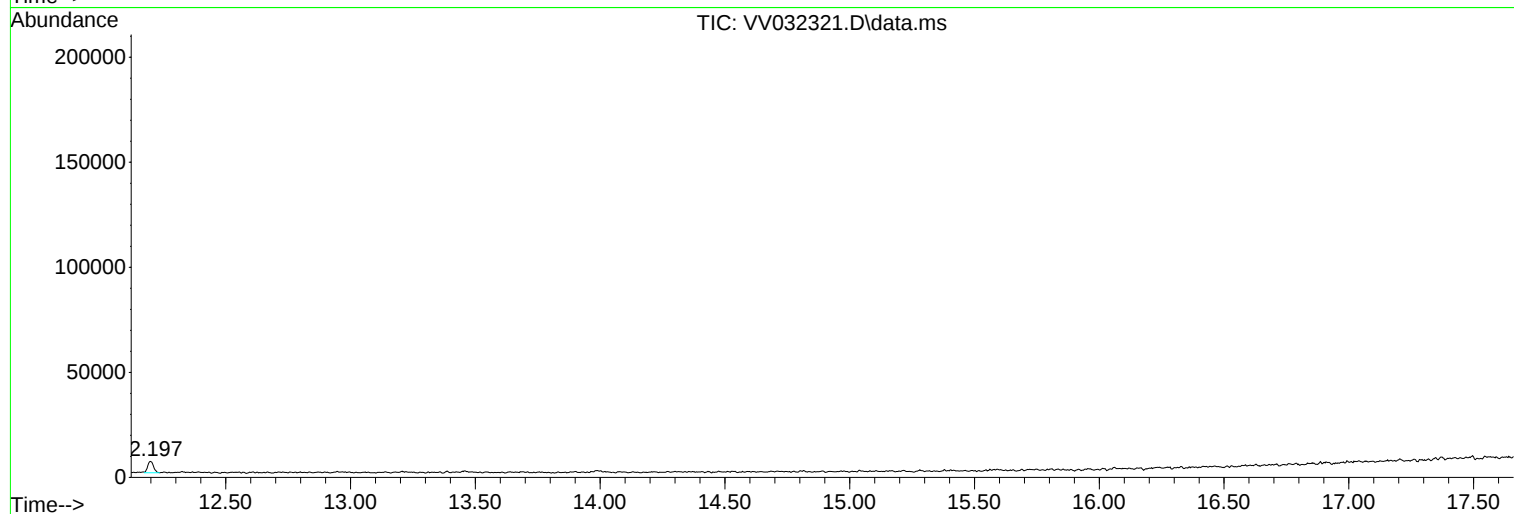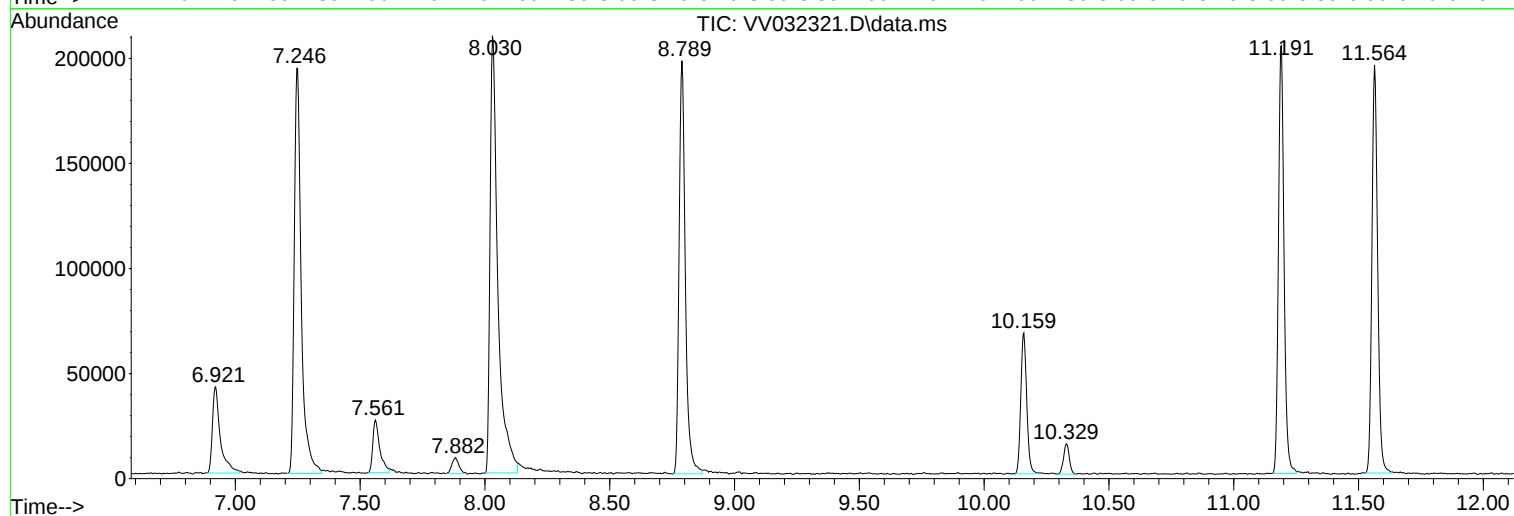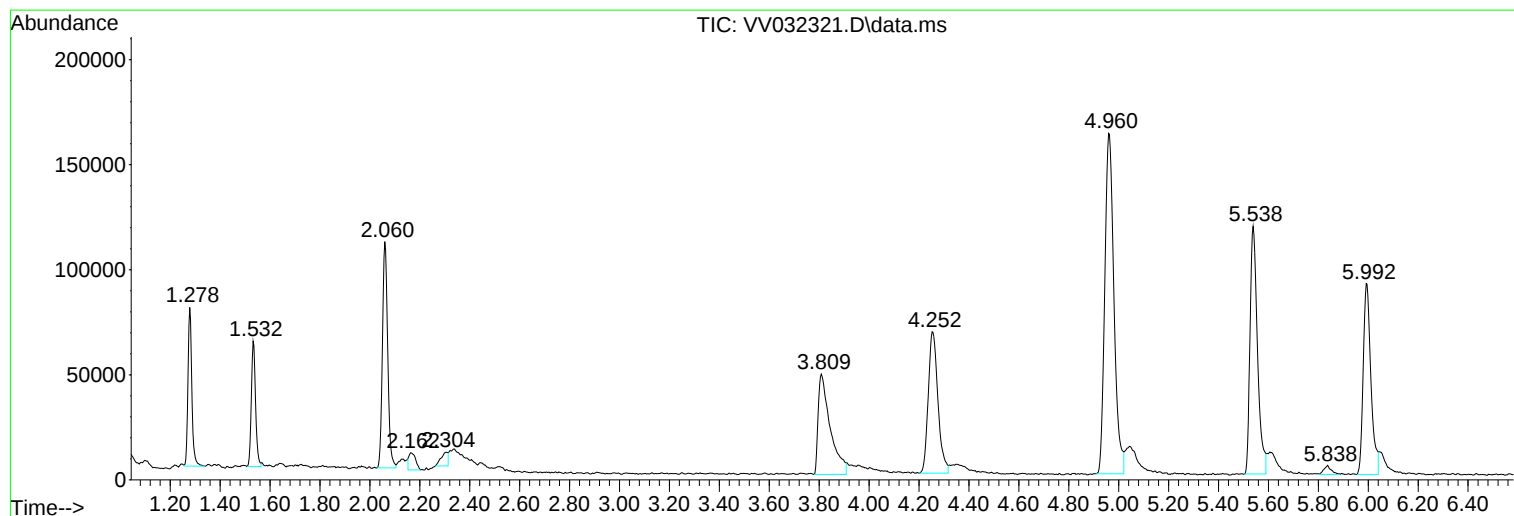

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032321.D
Acq On : 09 Oct 2023 12:09
Operator : SY/MD
Sample : 04708-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100923\
Data File : VV032321.D
Acq On : 09 Oct 2023 12:09
Operator : SY/MD
Sample : 04708-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc